

SUPERVISOR TEST




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906

Date: 07/28/2021

OPERATOR NAME:
ROBERT S CORNISH
Permit #: 48068
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:05
INTERNAL STANDARD	VERIFIED	22:05
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	22:06
BLANK TEST	0.00	22:07
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	22:07
BLANK TEST	0.00	22:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:08
BLANK TEST	0.00	22:09

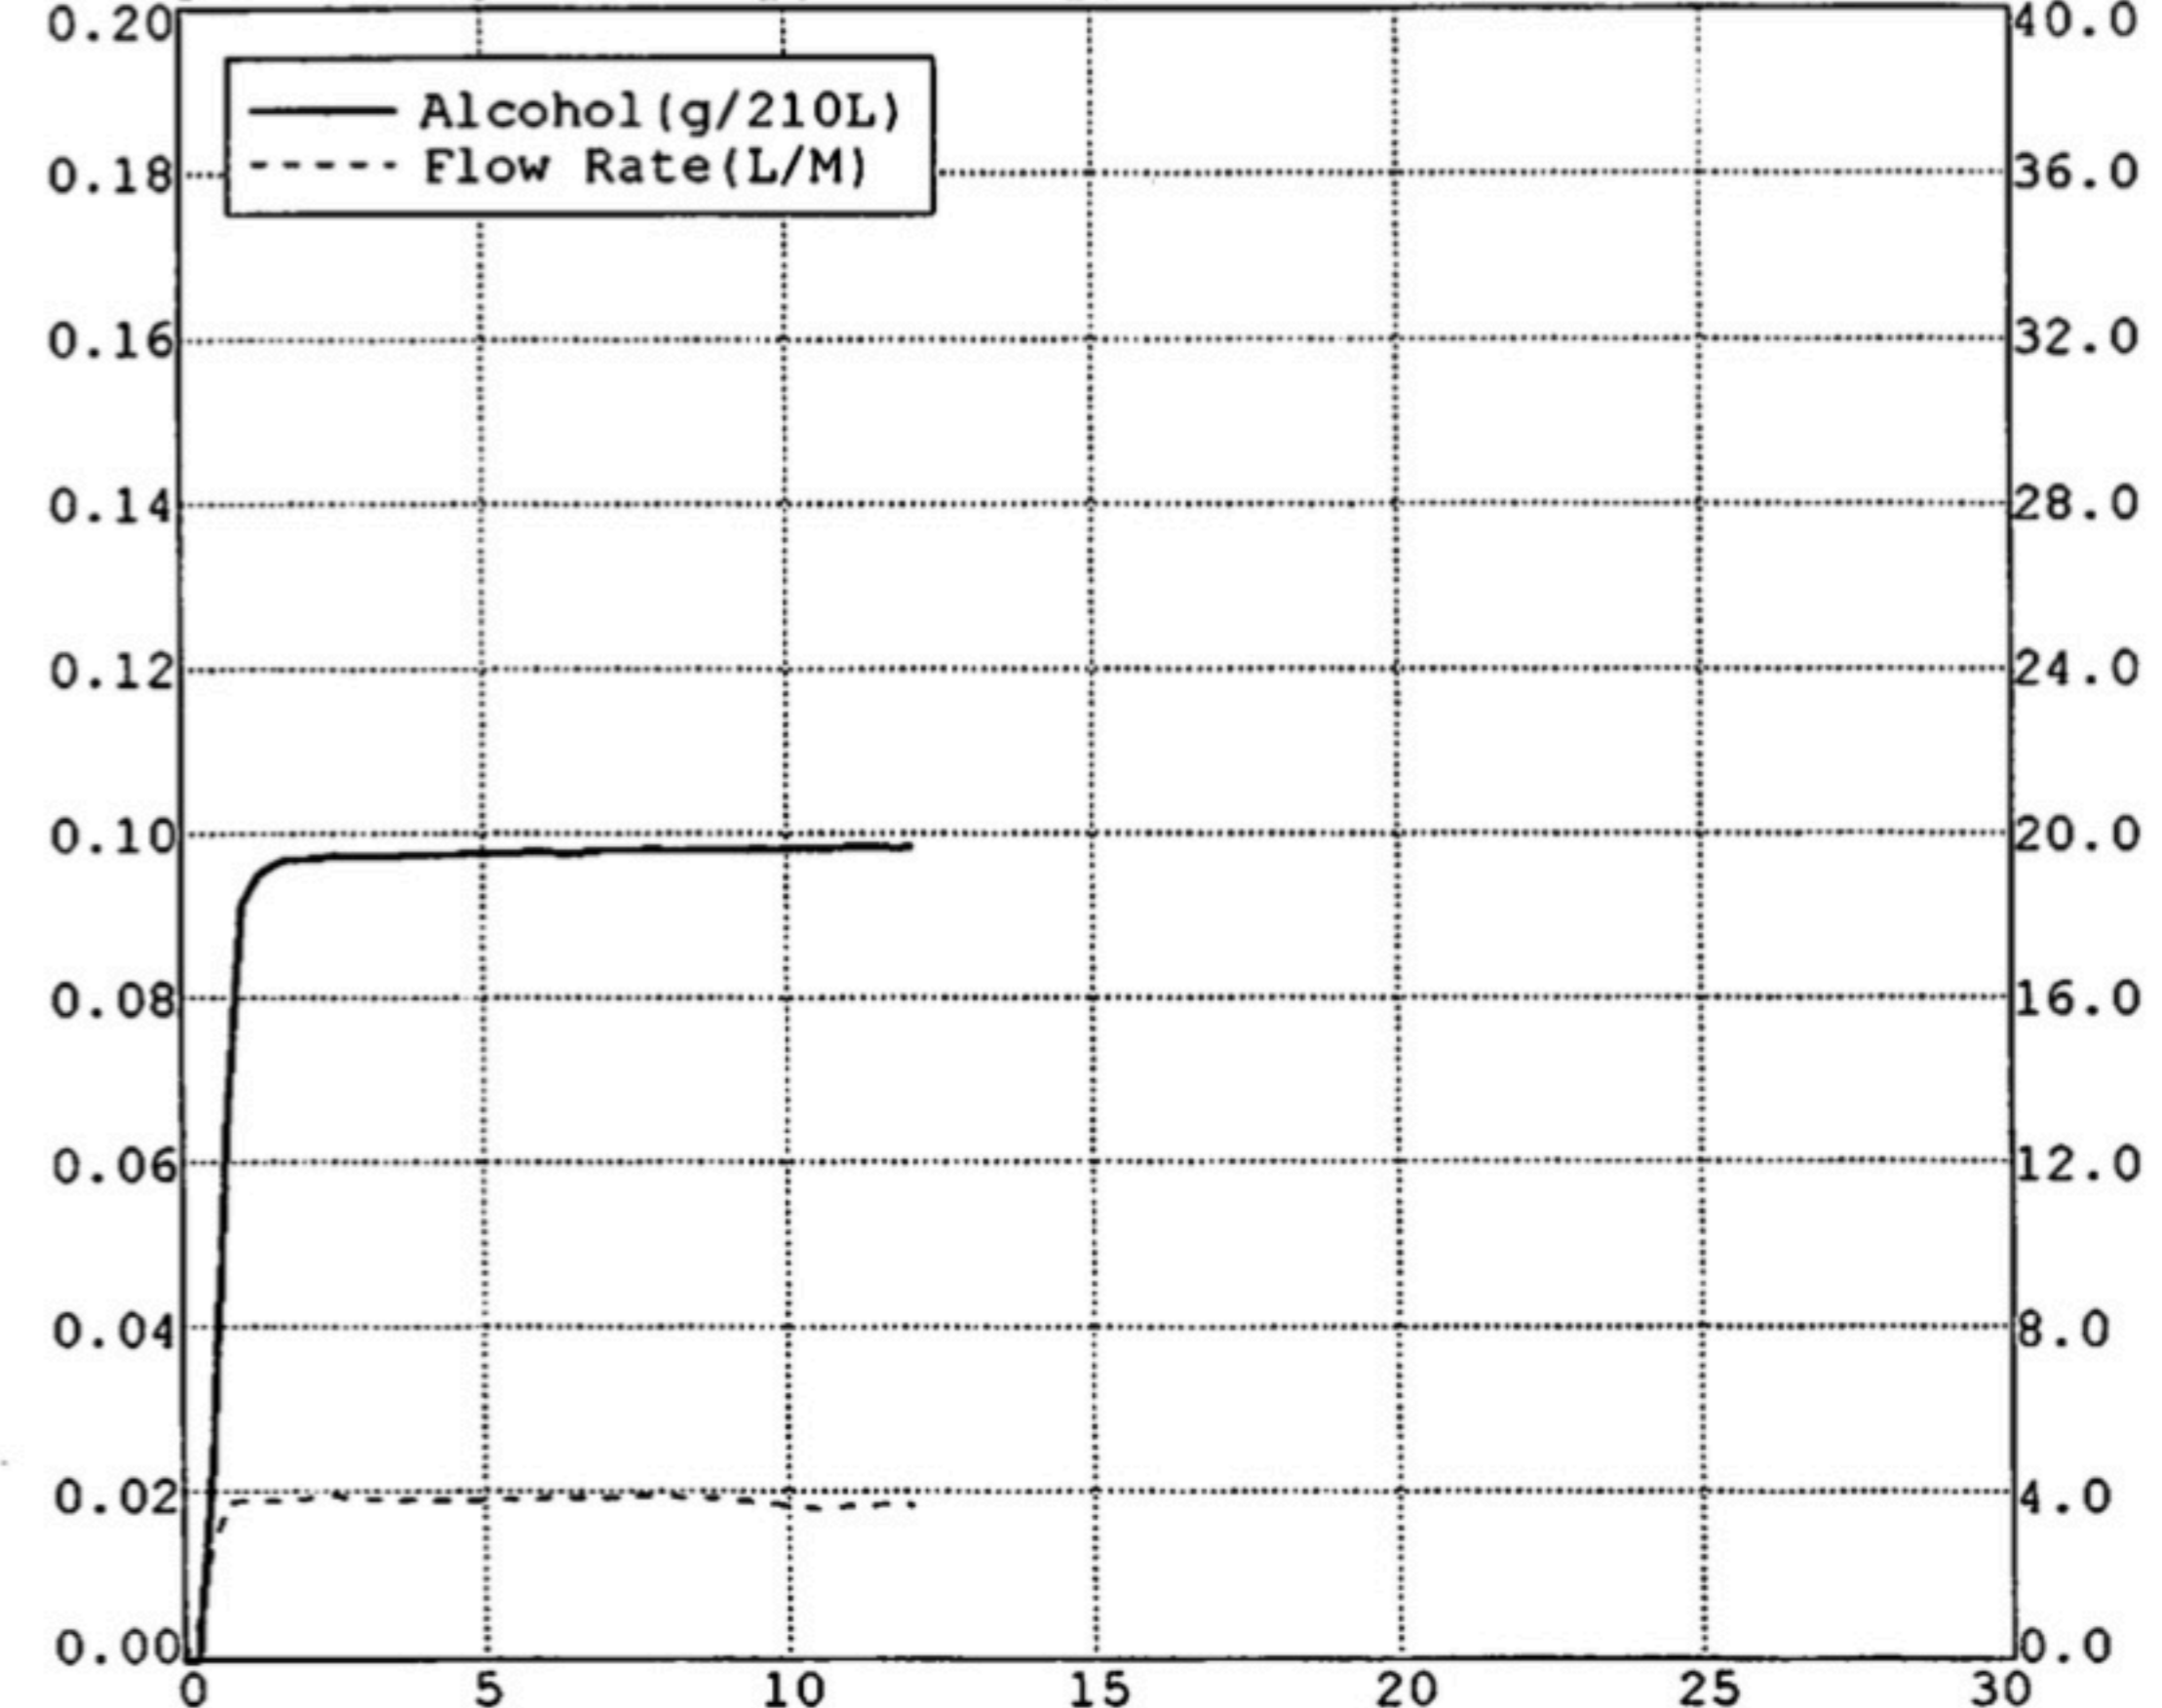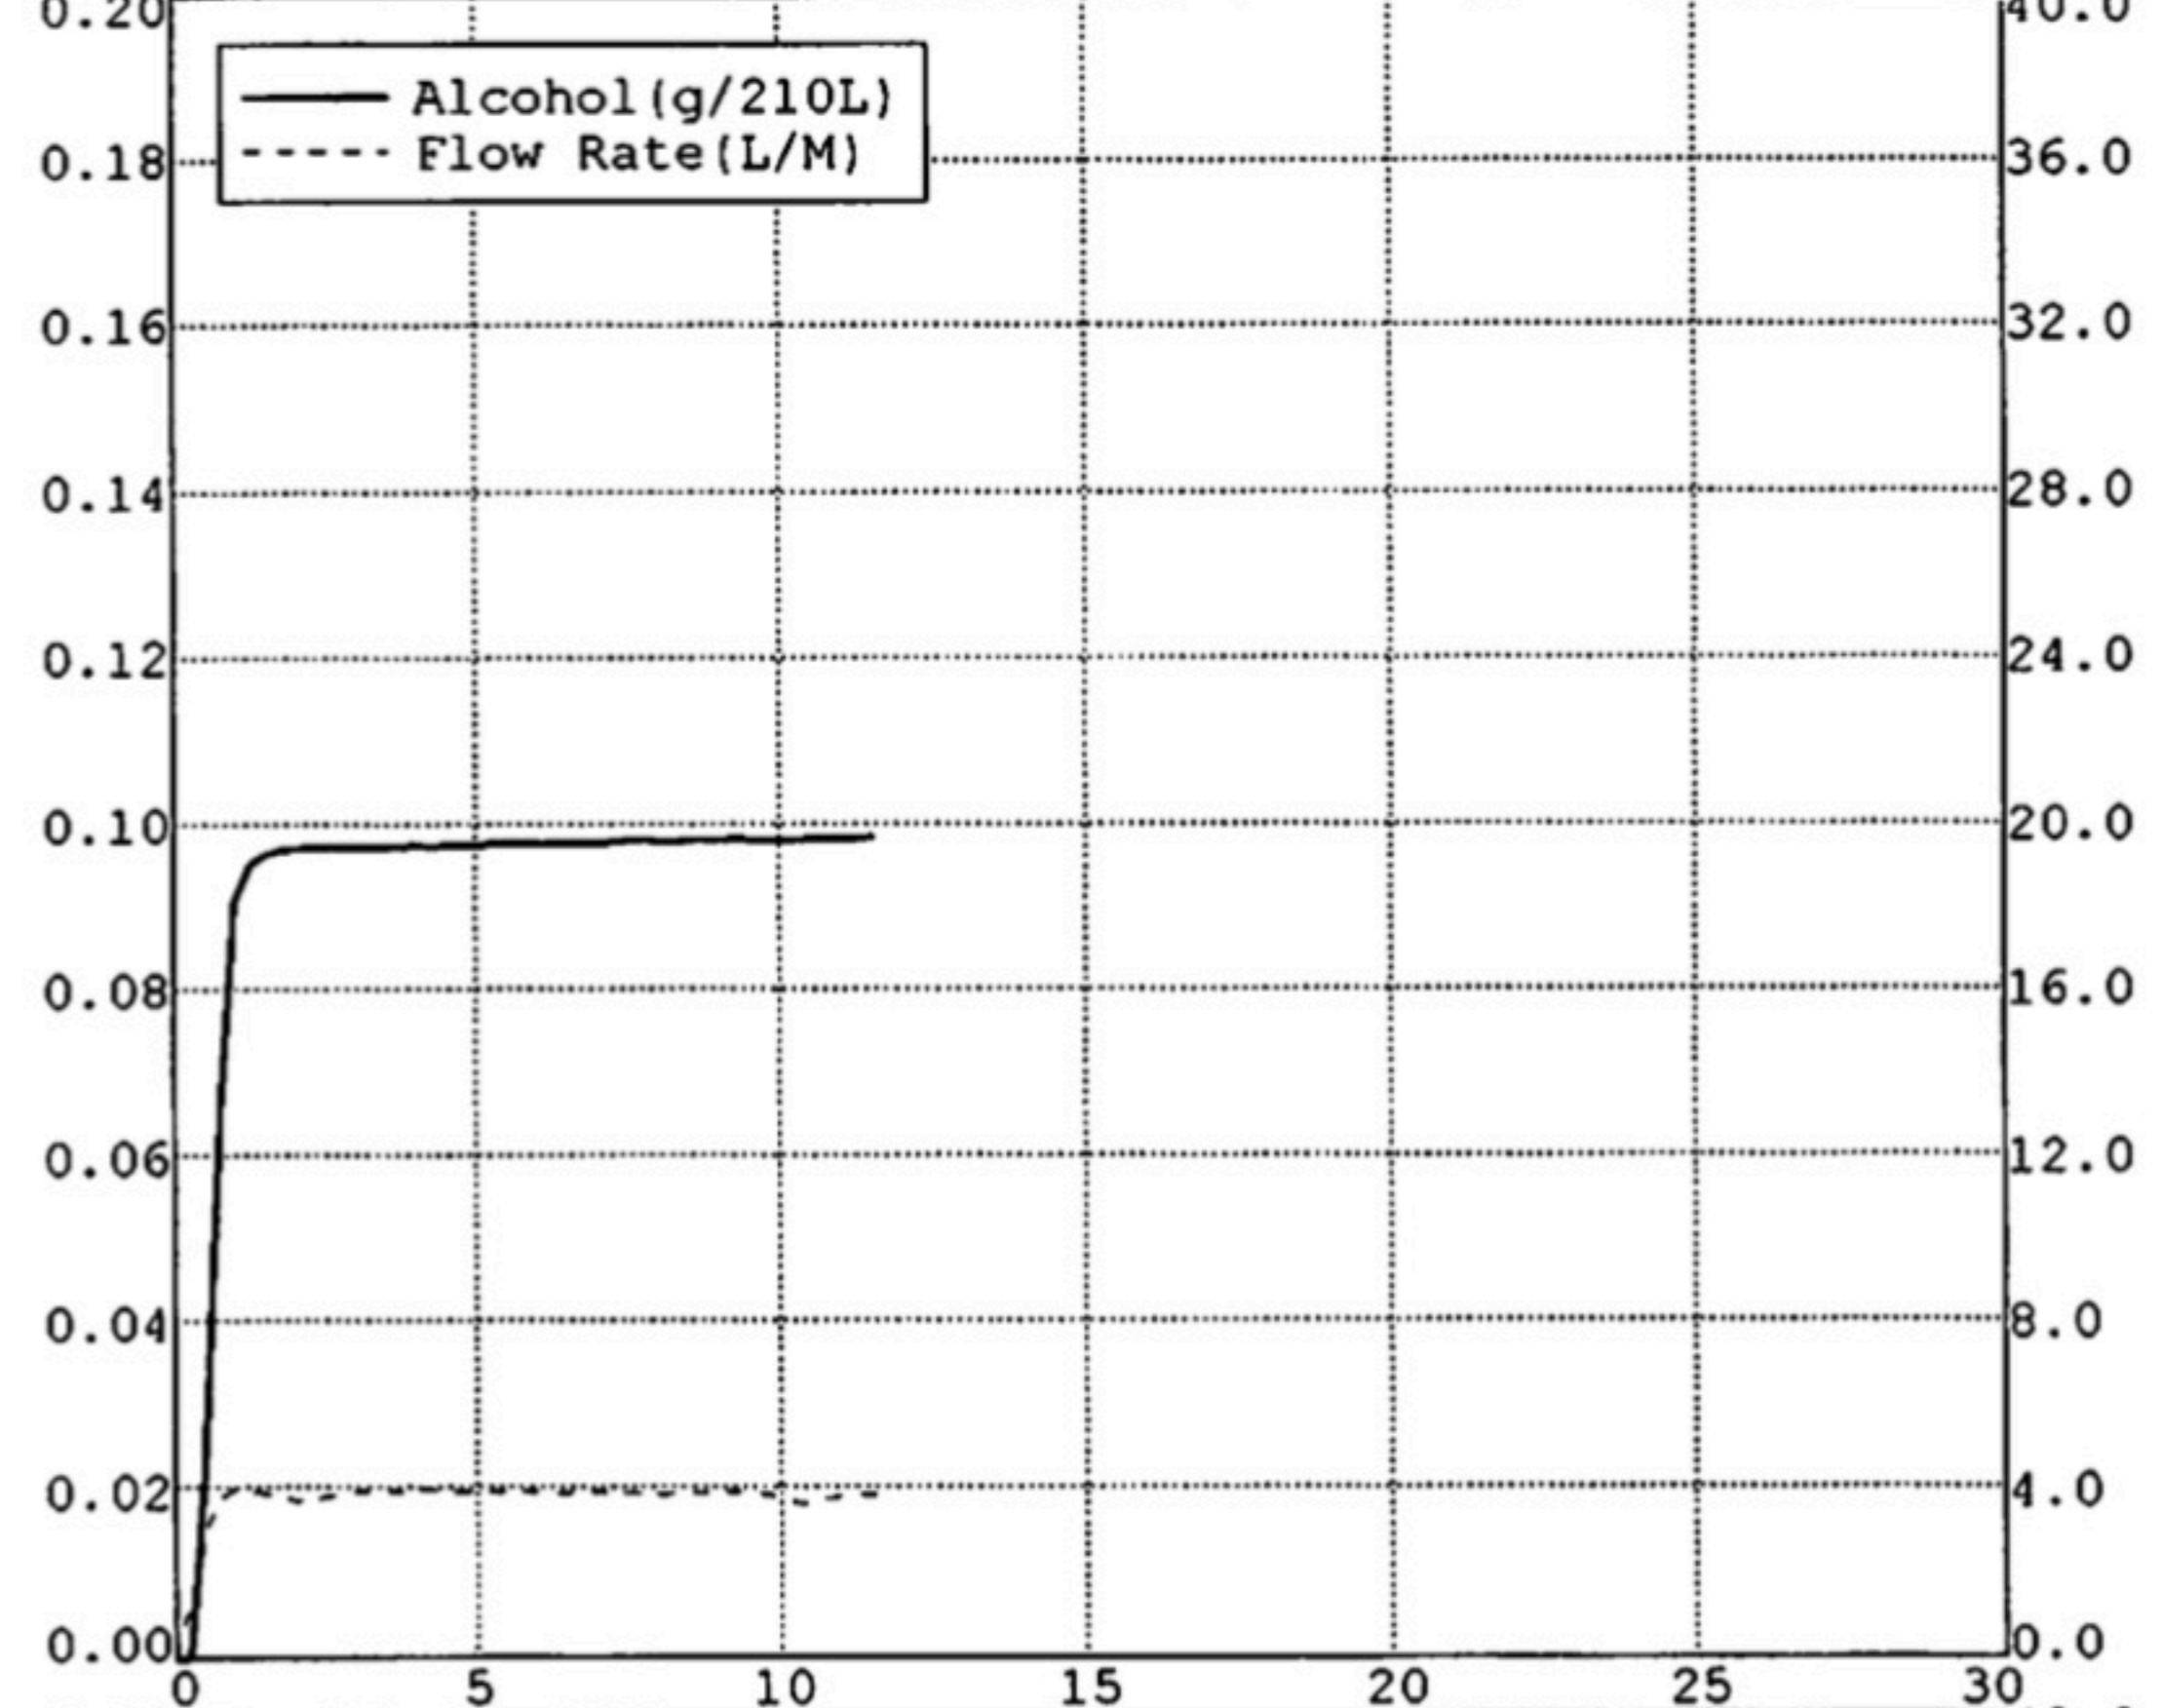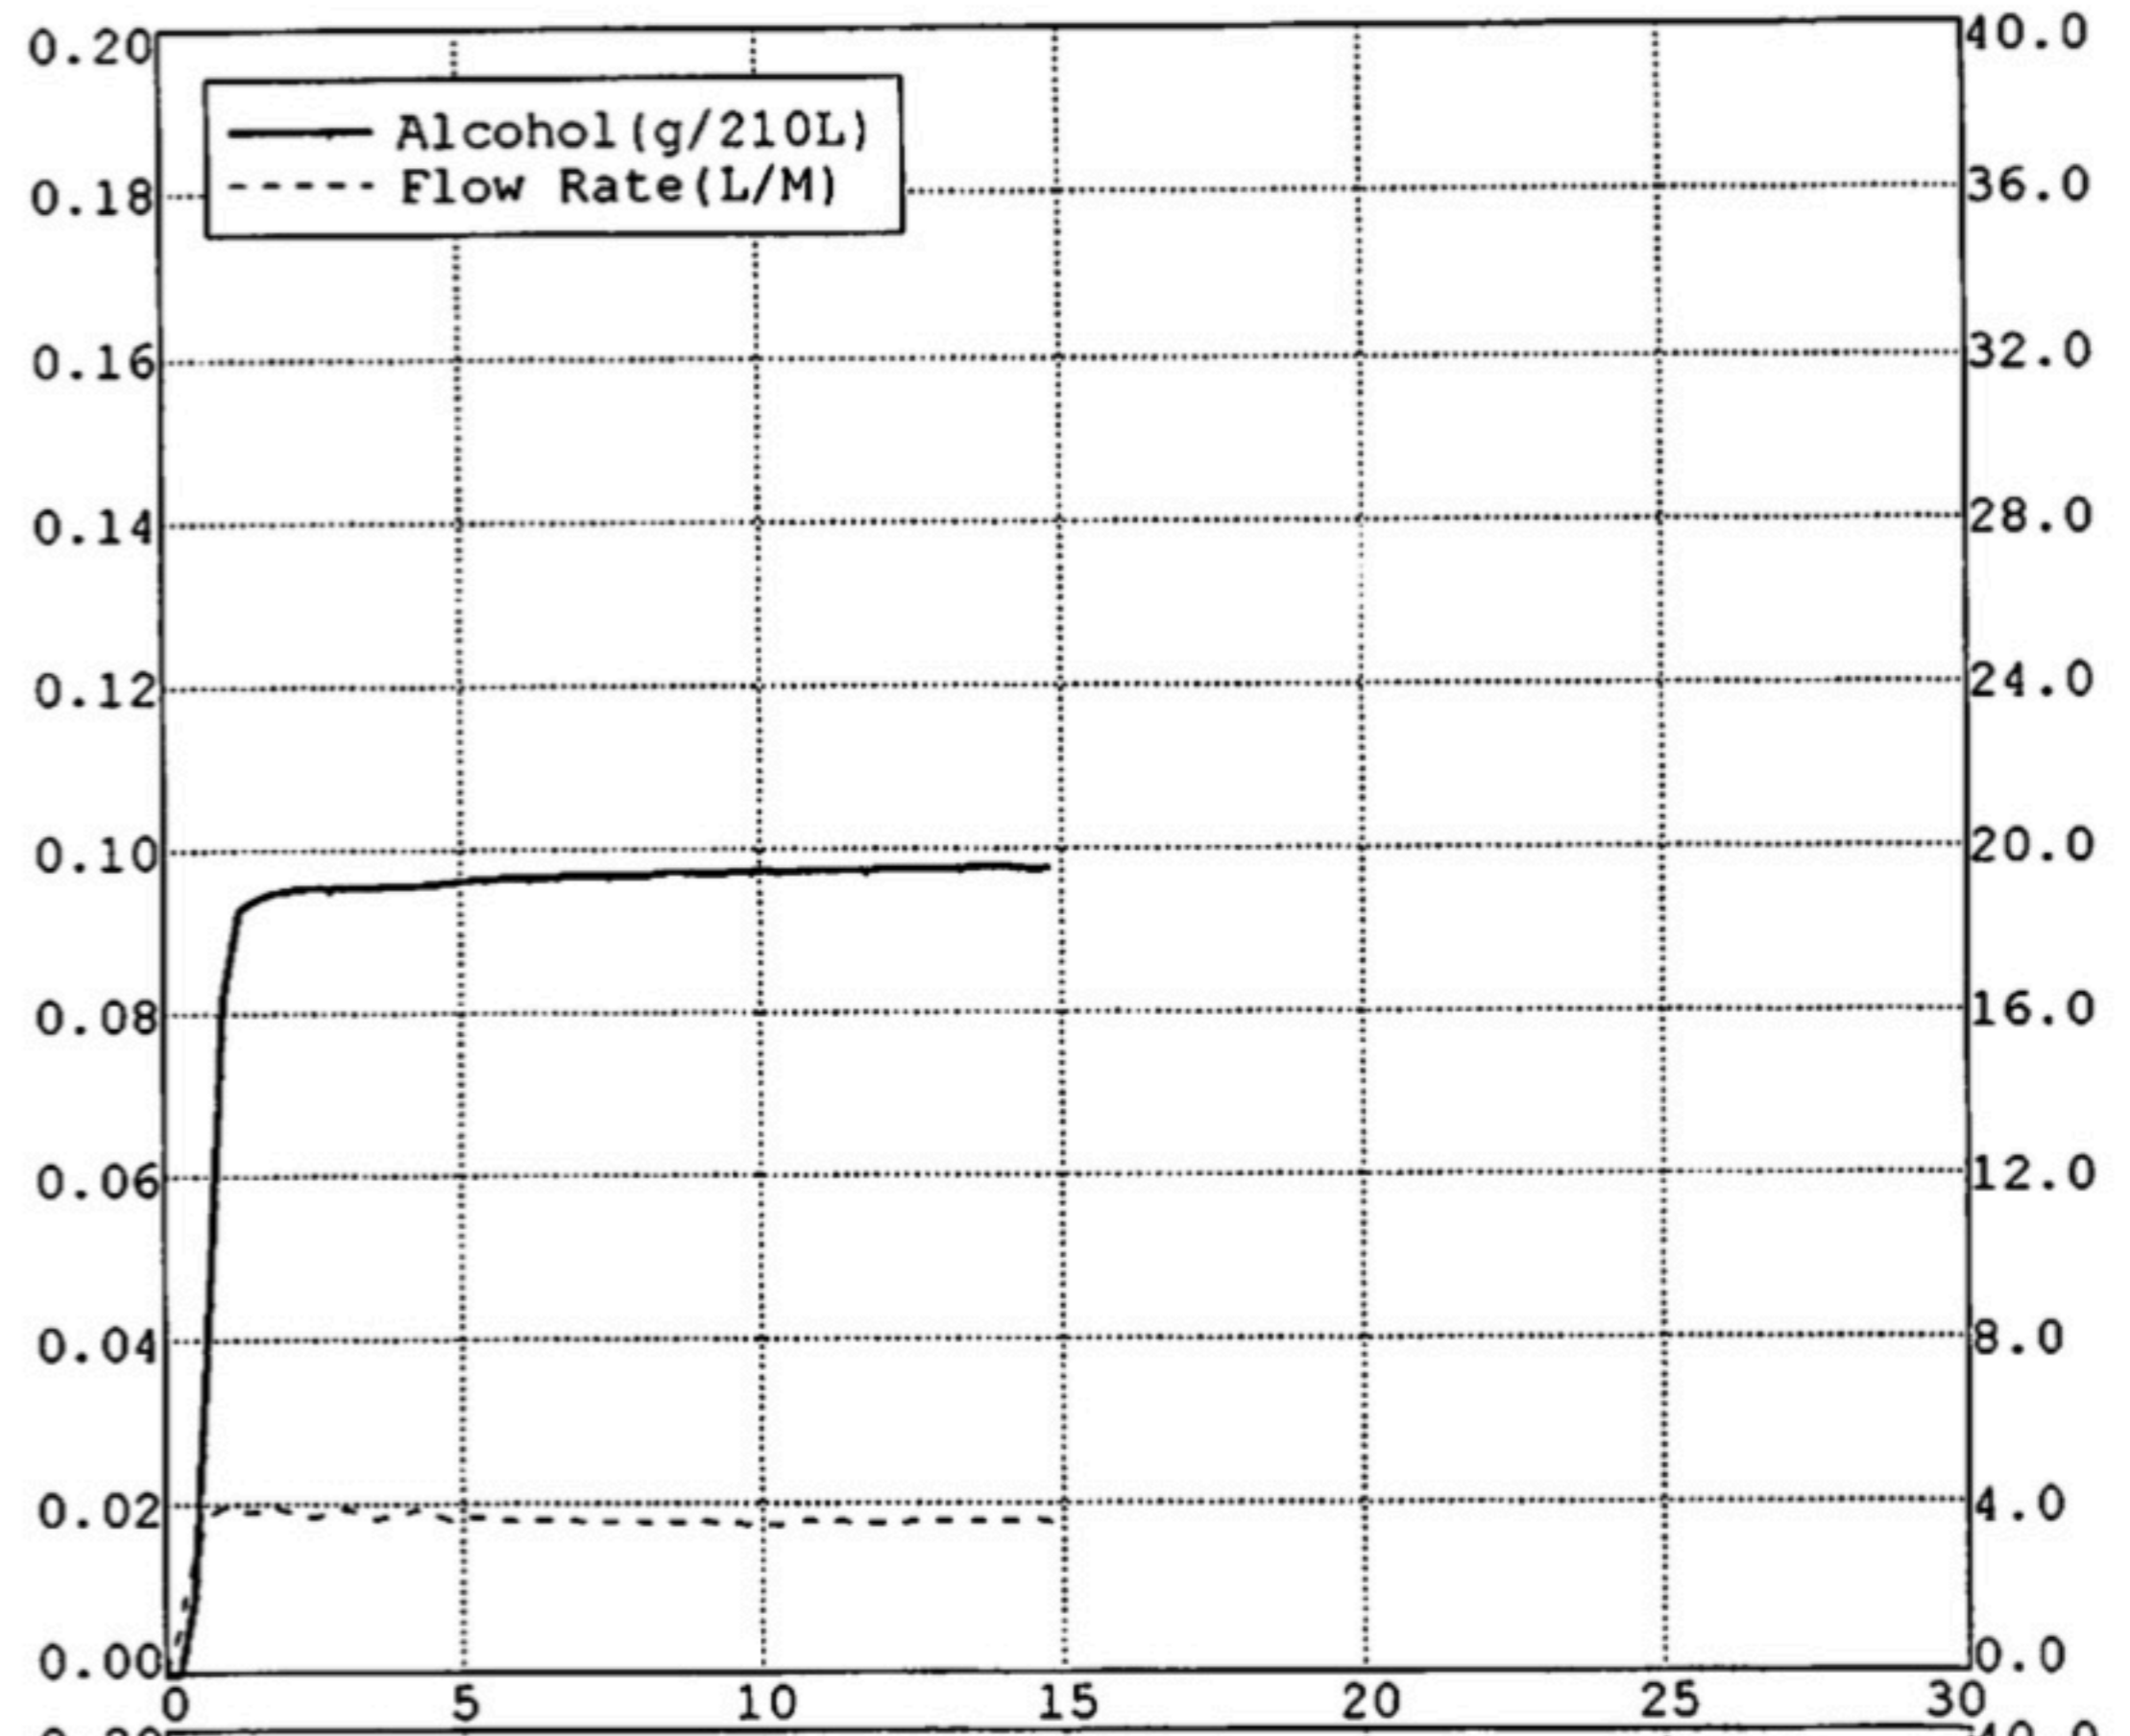

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906

Date: 08/04/2021

OPERATOR NAME:
STEVEN P EILERS
Permit #: 49321
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:01
INTERNAL STANDARD	VERIFIED	20:01
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	20:02
BLANK TEST	0.00	20:03
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	20:03
BLANK TEST	0.00	20:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	20:04
BLANK TEST	0.00	20:05

