

SUPERVISOR TEST



ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906

Date: 08/12/2021

OPERATOR NAME:
KRISTY N ALLEN
Permit #: 49726
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:58
INTERNAL STANDARD	VERIFIED	05:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	05:58
BLANK TEST	0.00	05:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	05:59
BLANK TEST	0.00	06:00
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	06:00
BLANK TEST	0.00	06:01

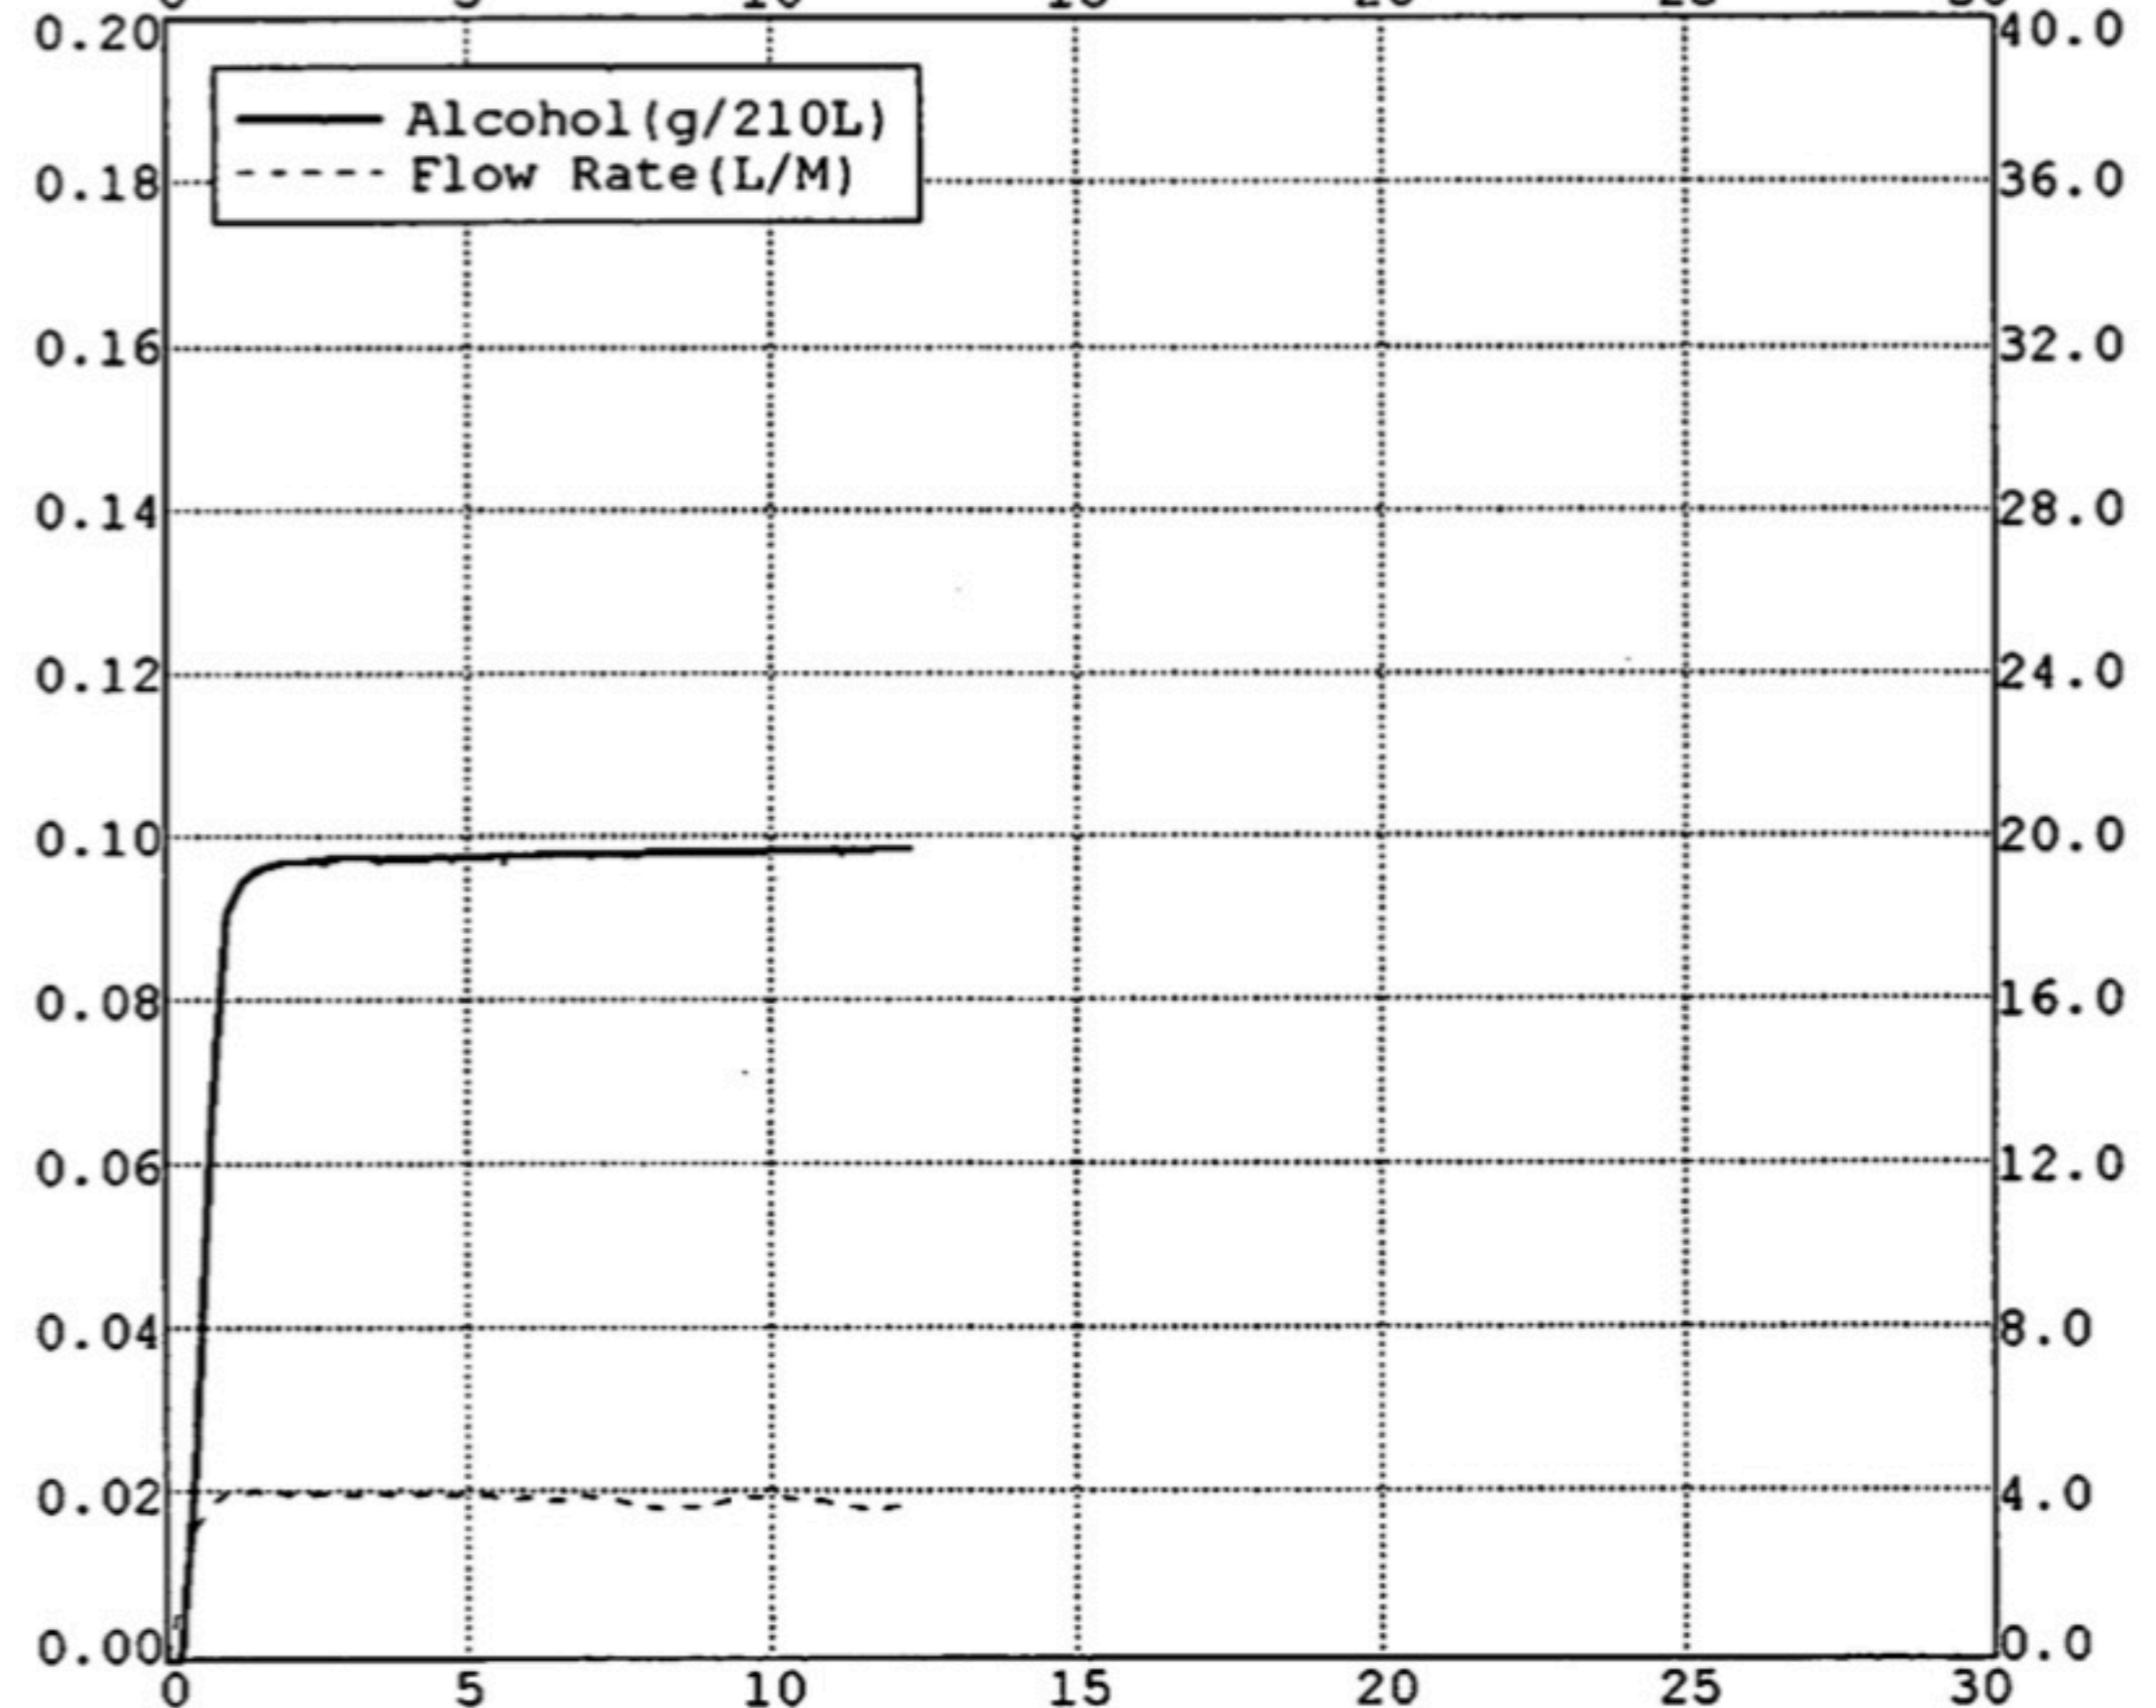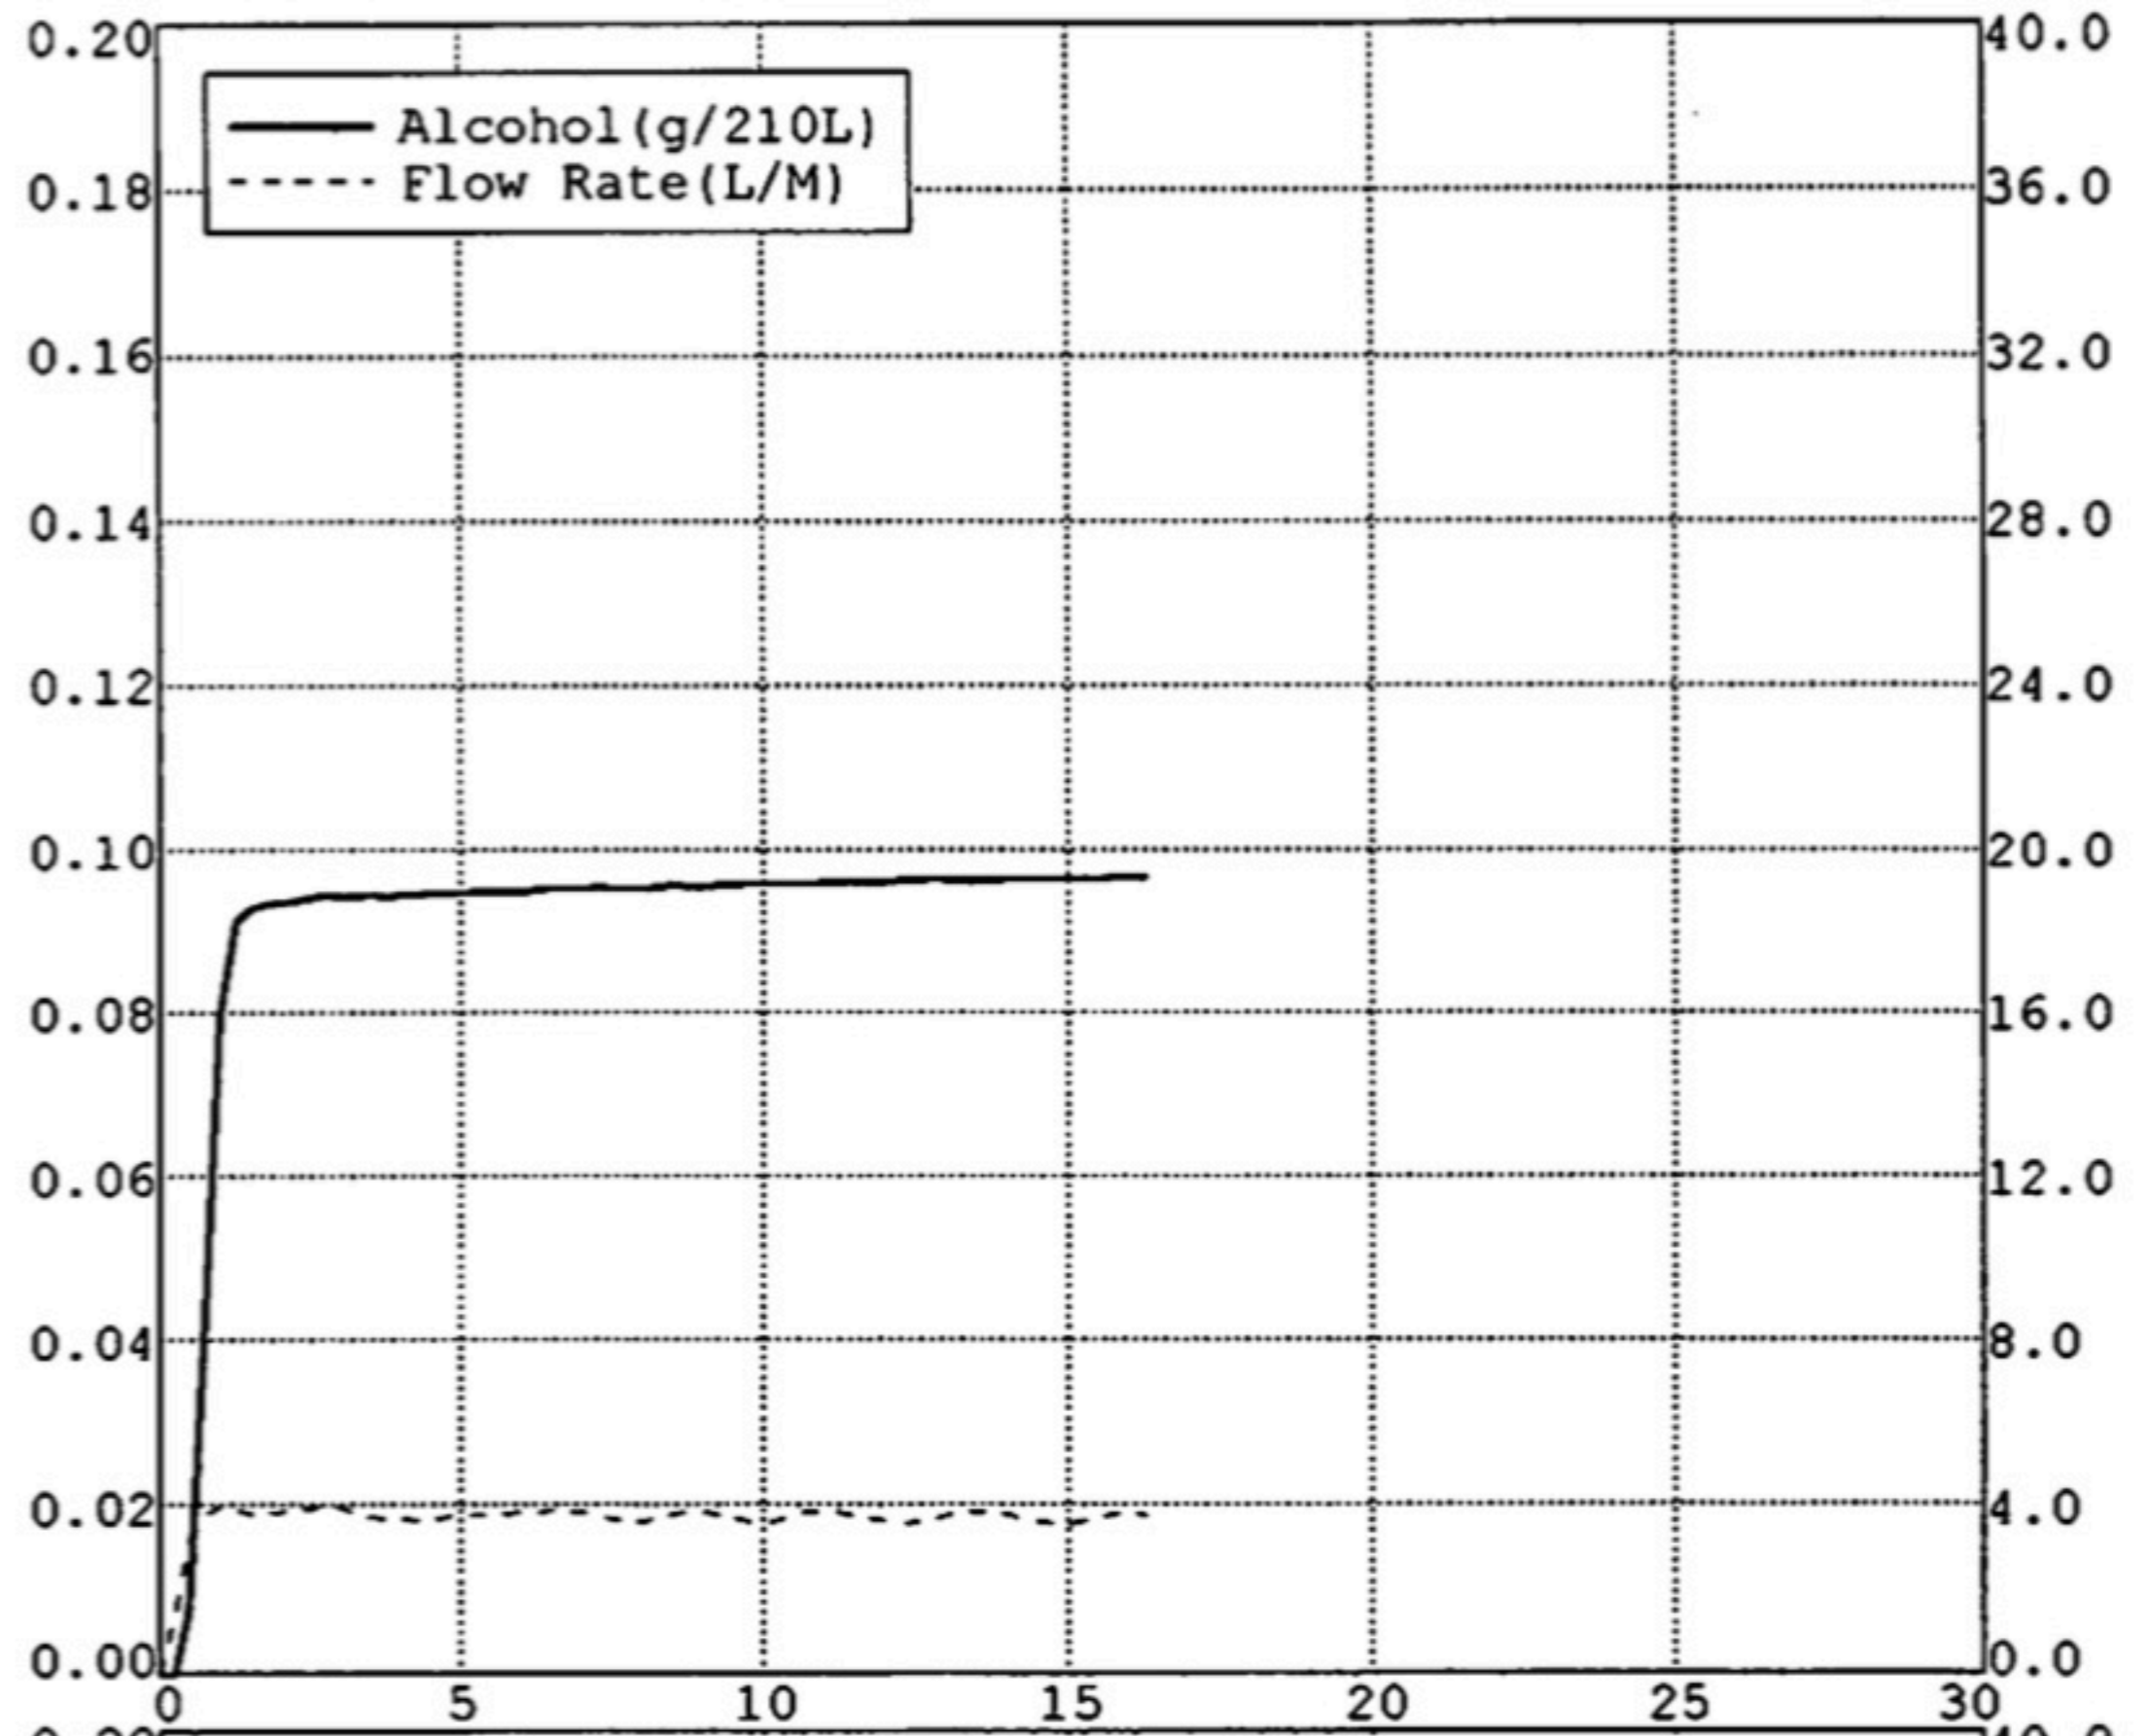

SUPERVISOR TEST




 ONEIDA COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 141906

Date: 08/12/2021

OPERATOR NAME:
 KRISTY N ALLEN
 Permit #: 49726
 Operator Agency/Dept: ONEIDA CO. S.O.
 Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:58
INTERNAL STANDARD	VERIFIED	05:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	05:58
BLANK TEST	0.00	05:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	05:59
BLANK TEST	0.00	06:00
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	06:00
BLANK TEST	0.00	06:01

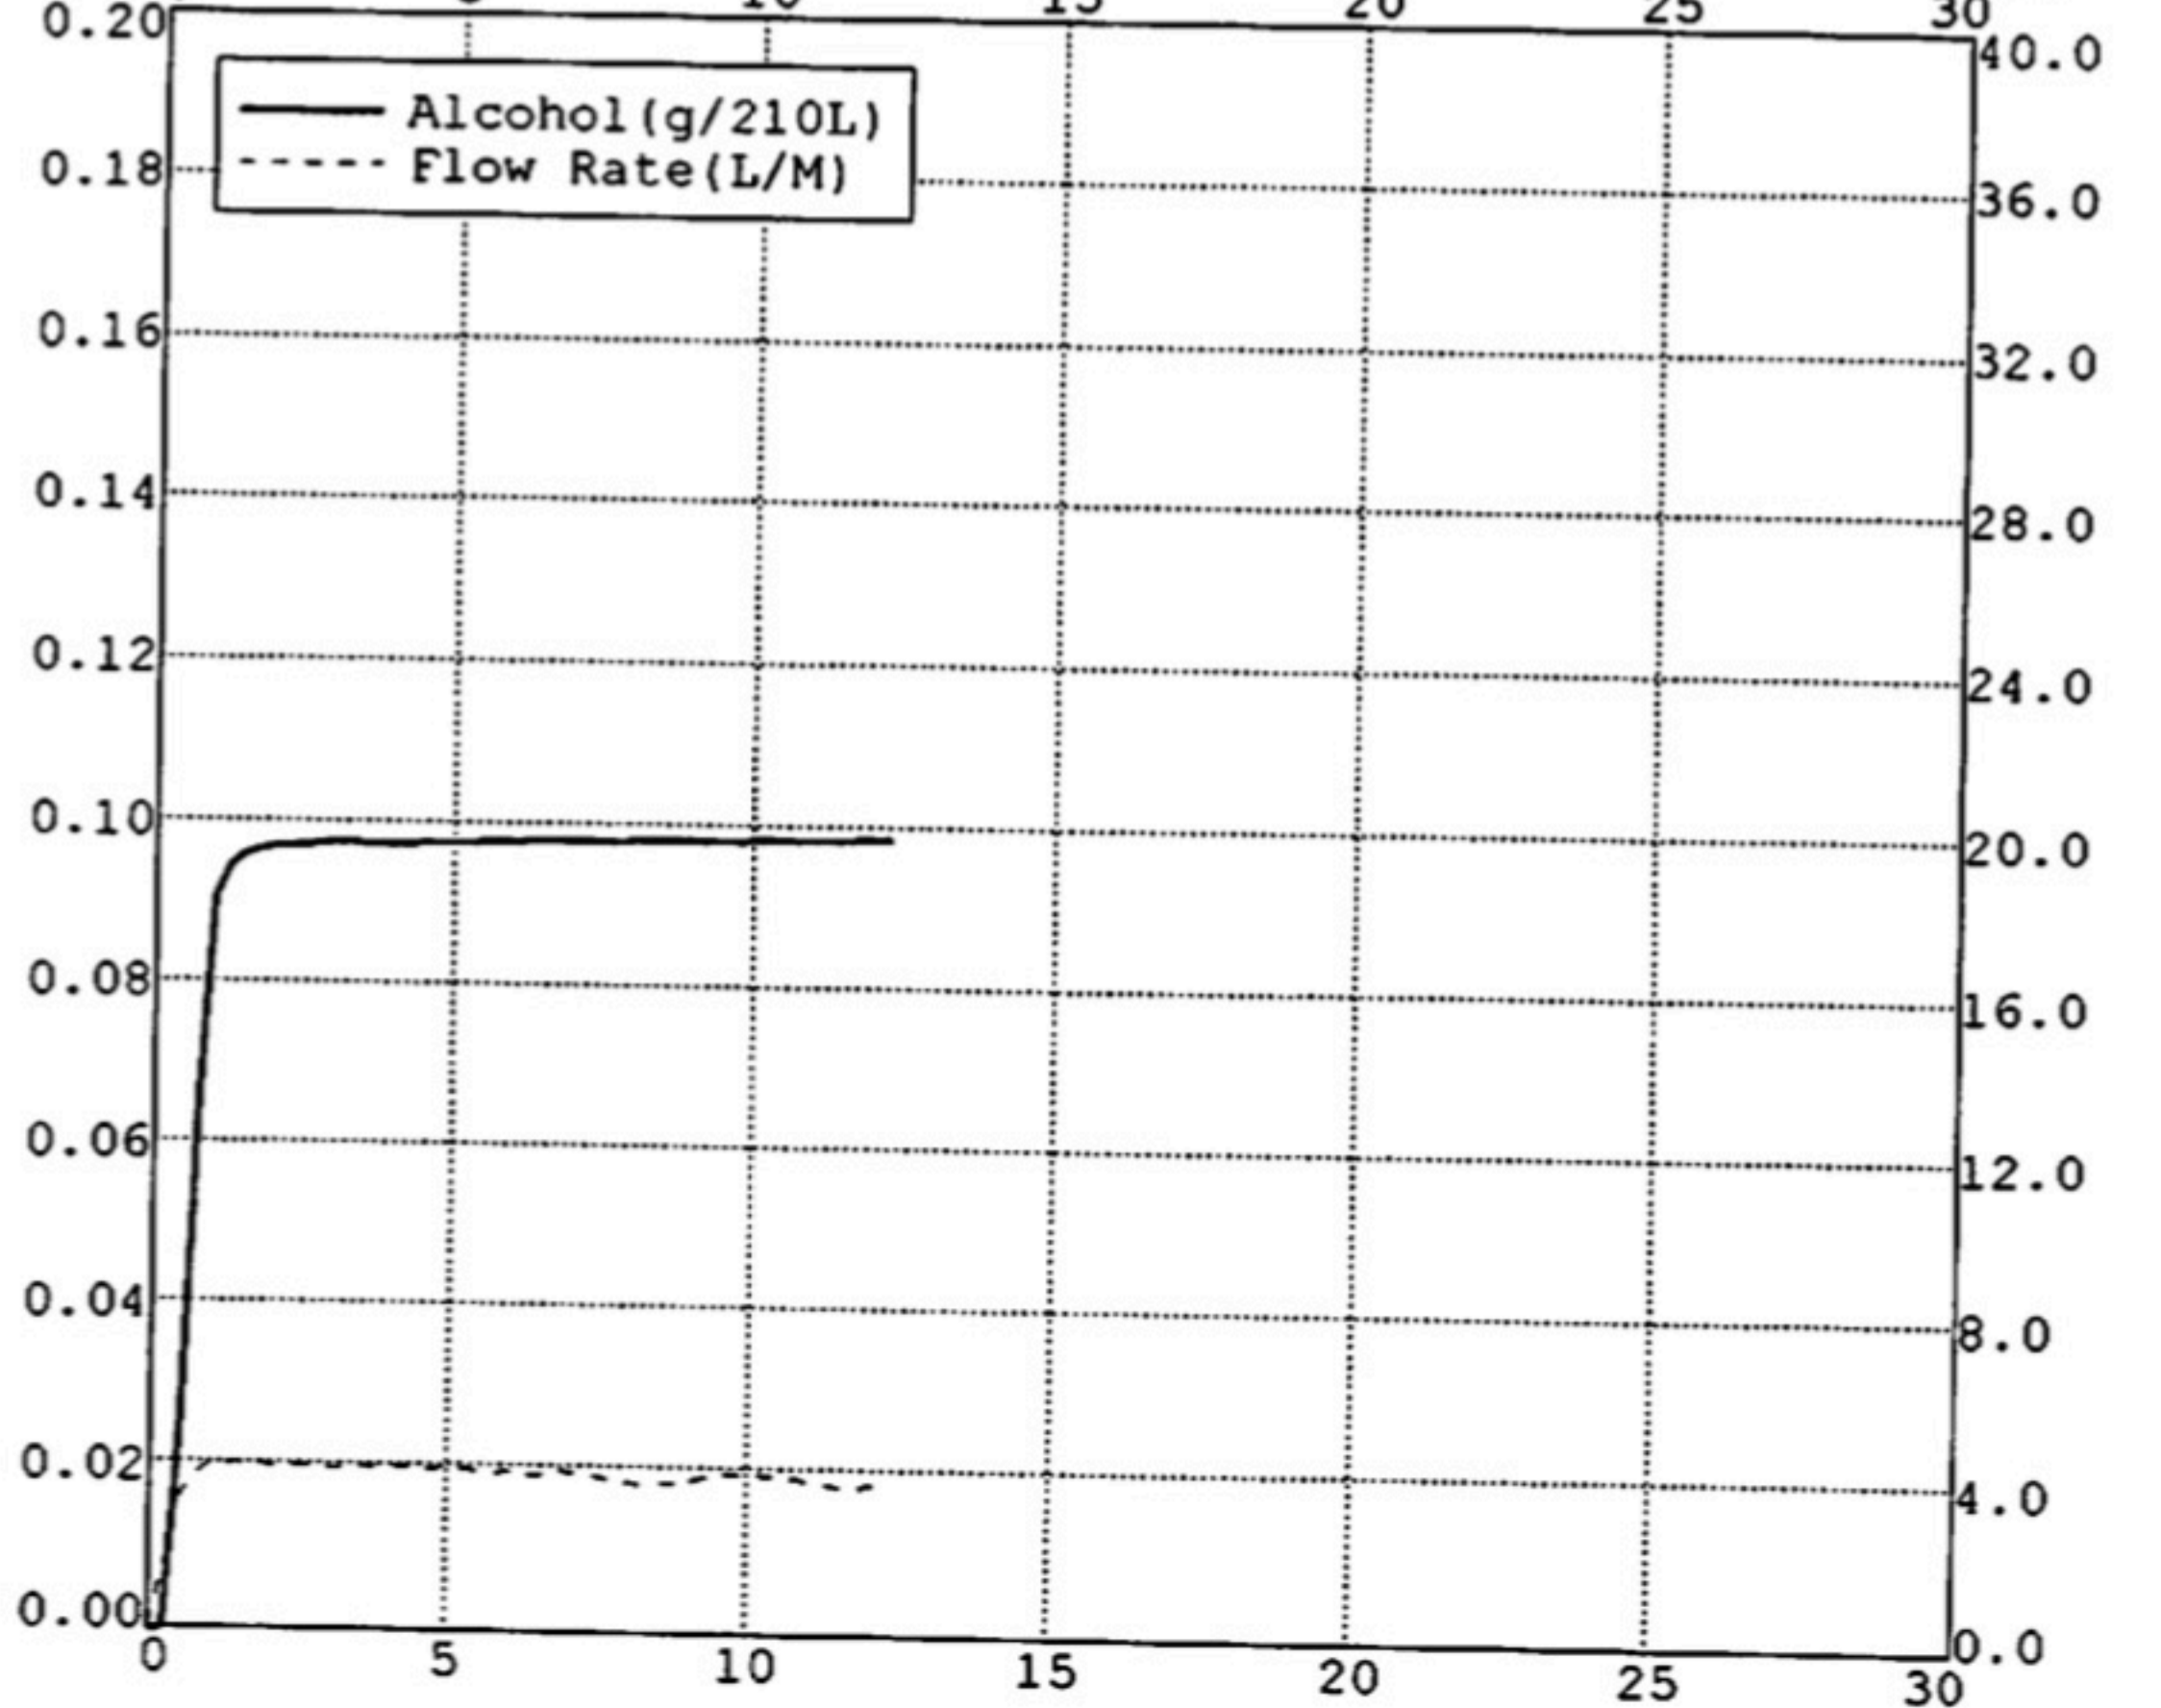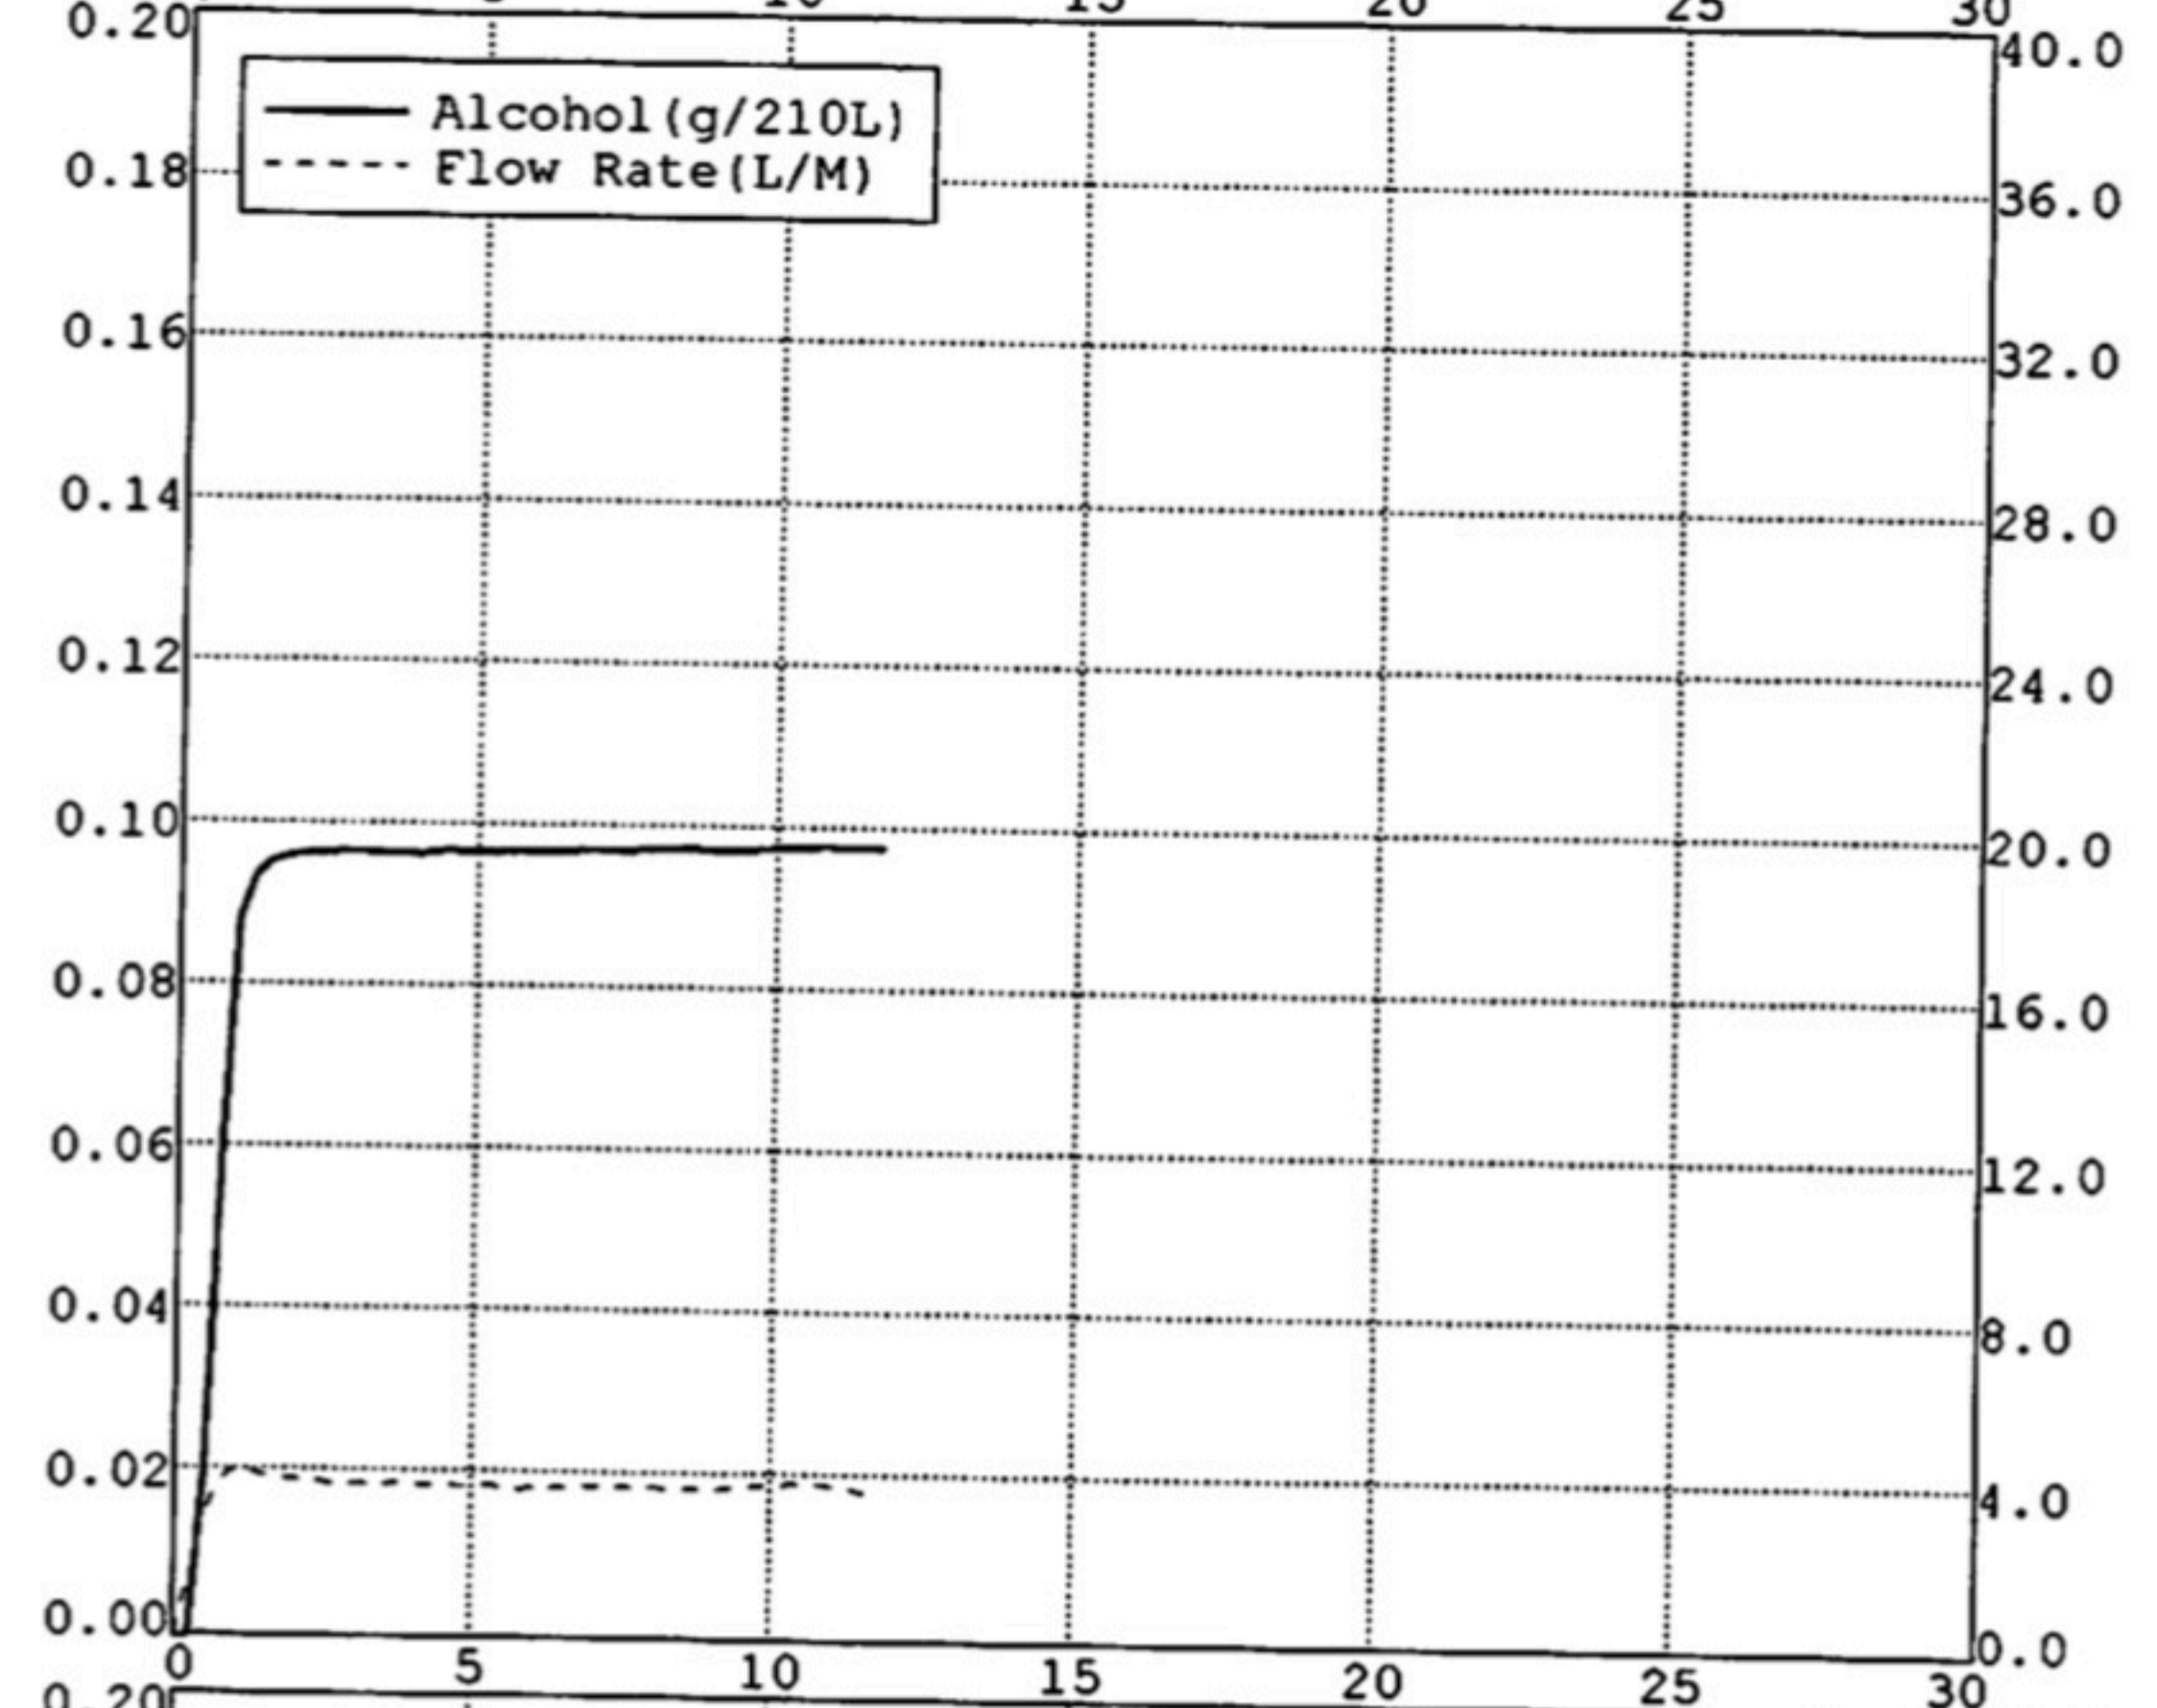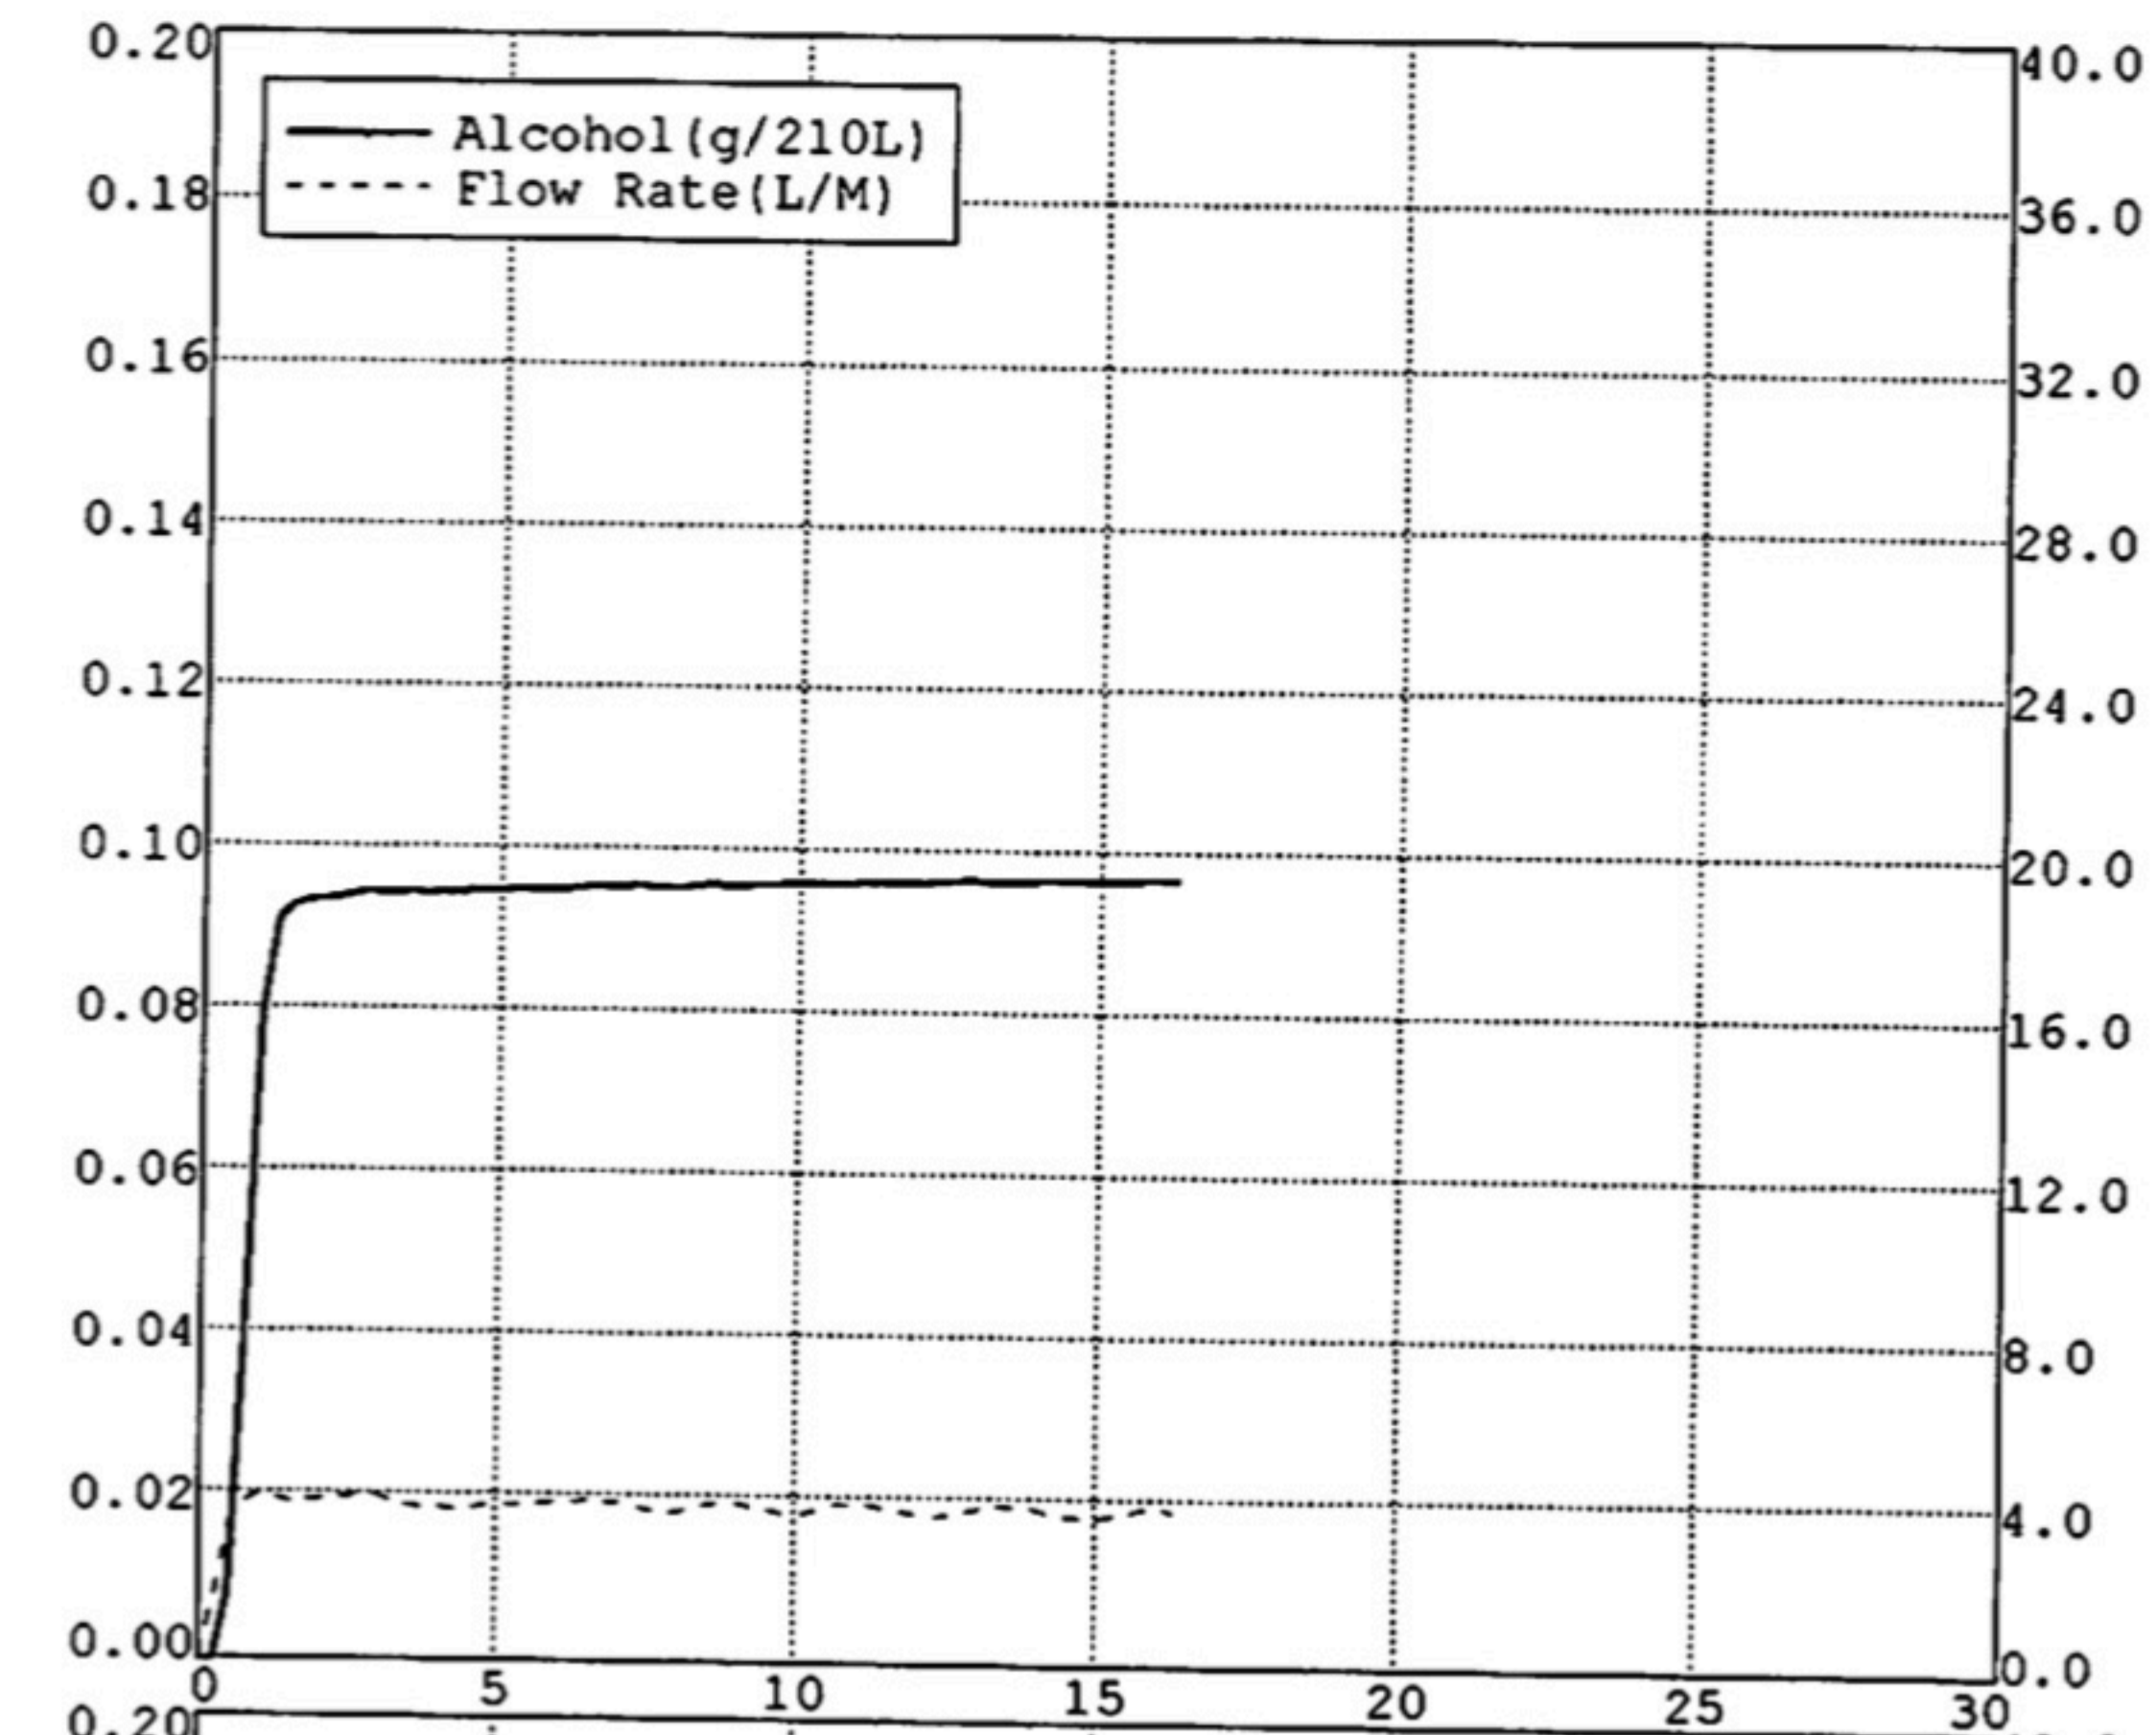

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906

Date: 08/18/2021

OPERATOR NAME:
JASON L OSIKA
Permit #: 35567
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:29
INTERNAL STANDARD	VERIFIED	20:29
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	20:30
BLANK TEST	0.00	20:31
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	20:31
BLANK TEST	0.00	20:32
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	20:32
BLANK TEST	0.00	20:33

