

SUPERVISOR TEST

BFD




ONEIDA COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 141906

Date: 04/12/2023

OPERATOR NAME:
 JASON L OSIKA
 Permit #: 35567
 Operator Agency/Dept: ONEIDA CO. S.O.
 Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:04
INTERNAL STANDARD	VERIFIED	03:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	03:05
BLANK TEST	0.00	03:05
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	03:06
BLANK TEST	0.00	03:07
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	03:07
BLANK TEST	0.00	03:08

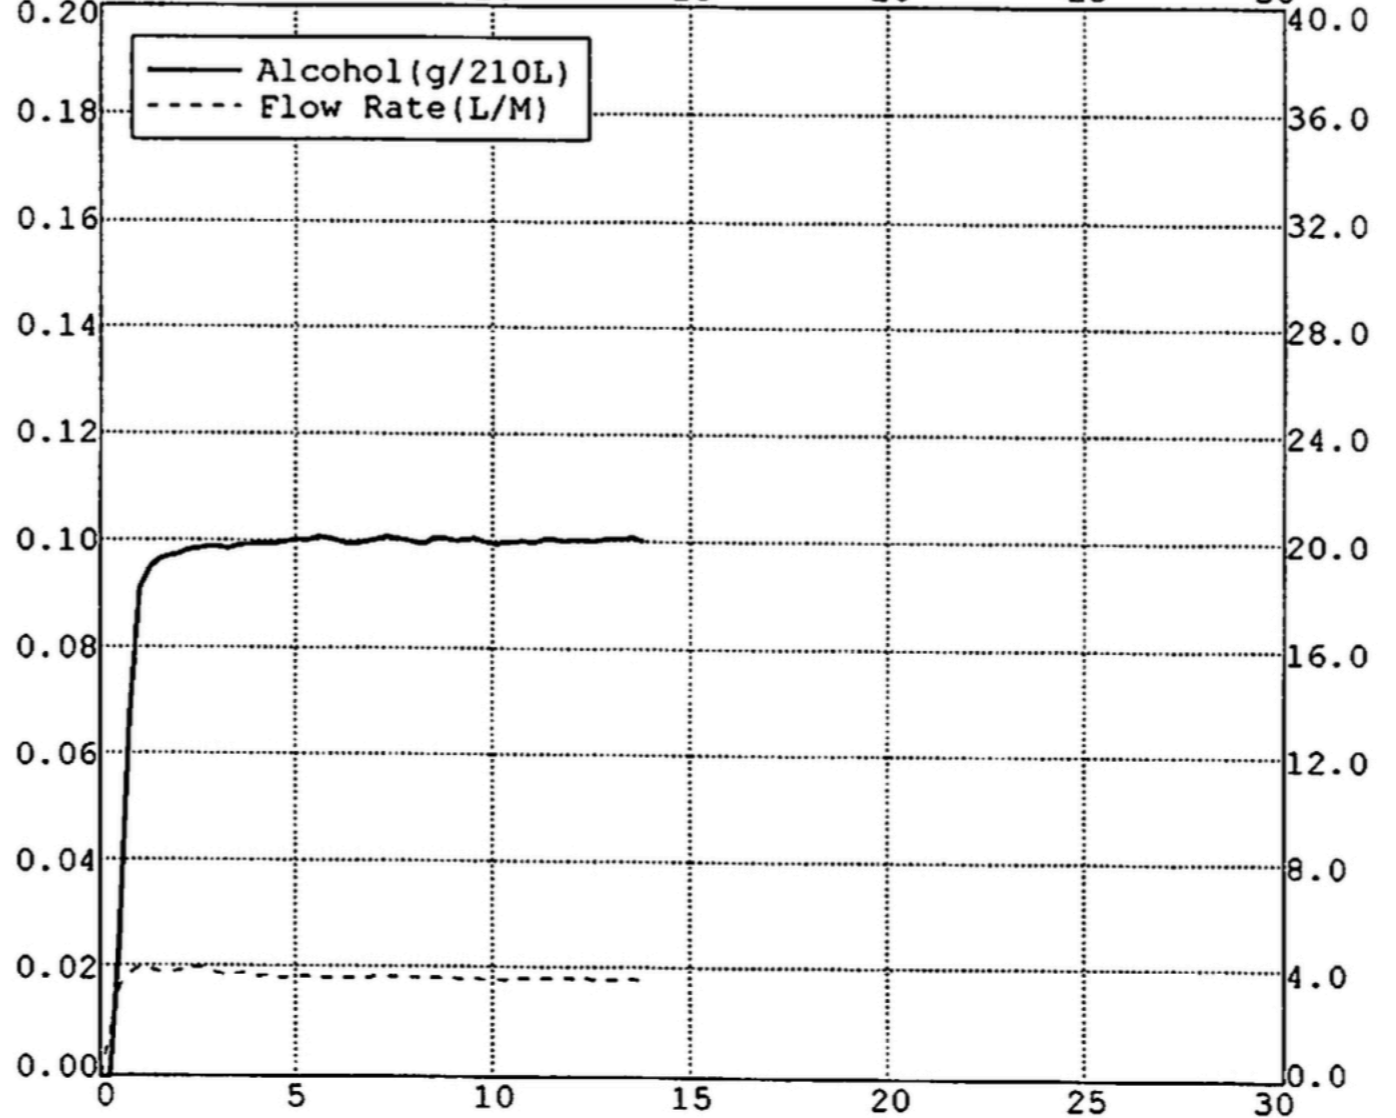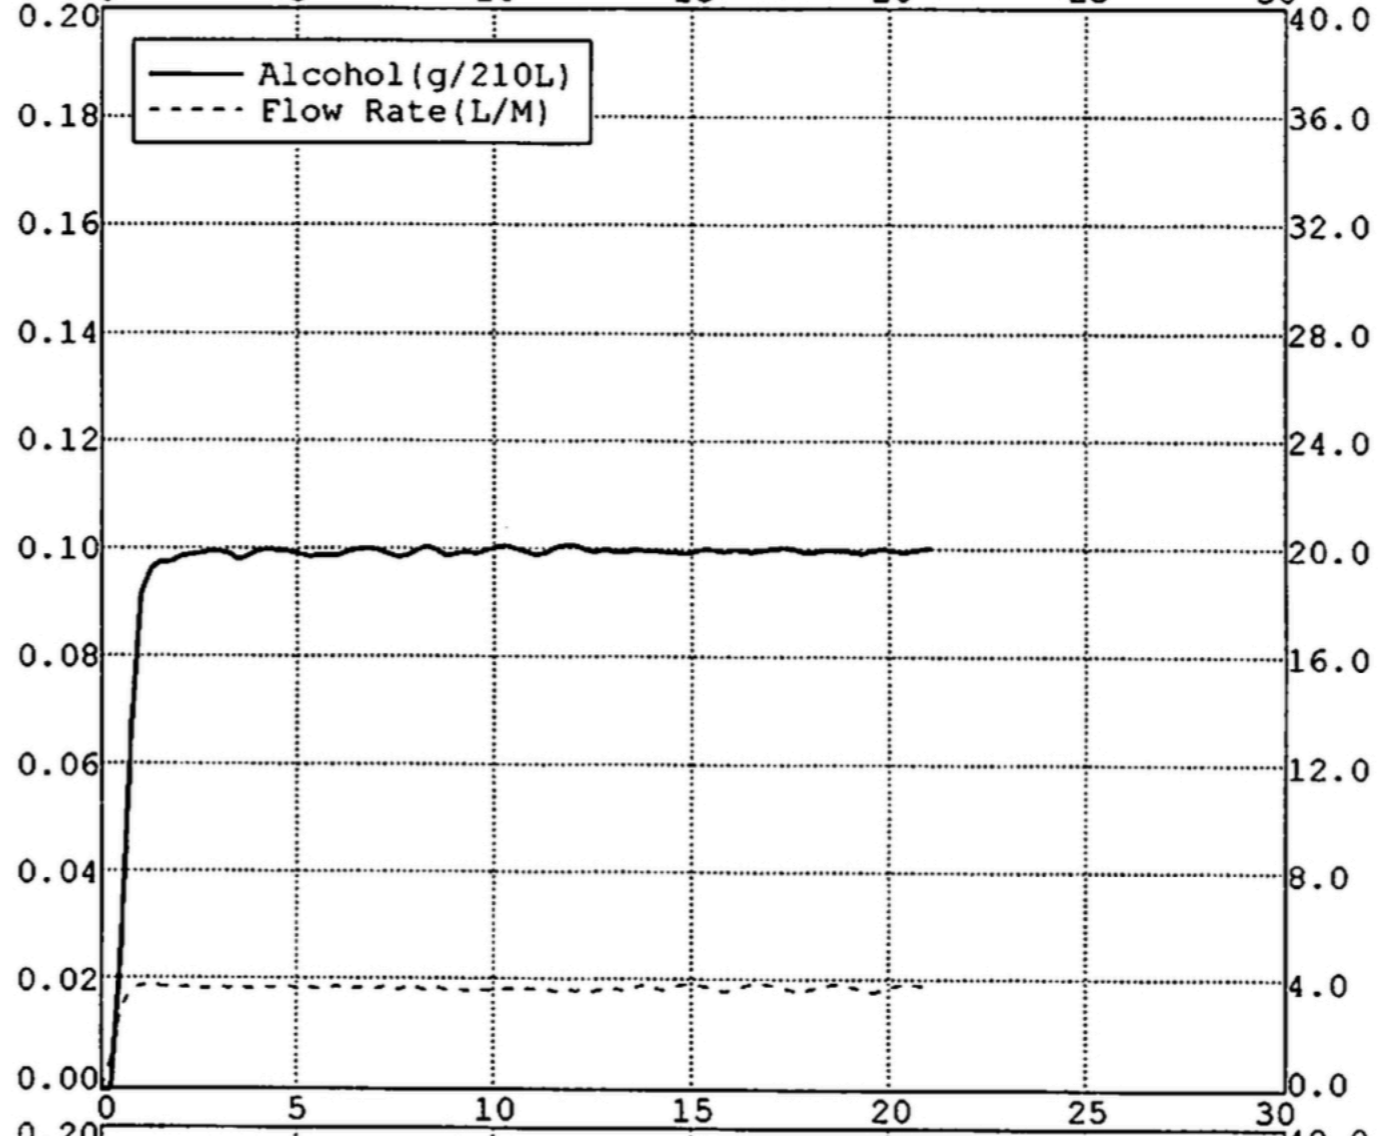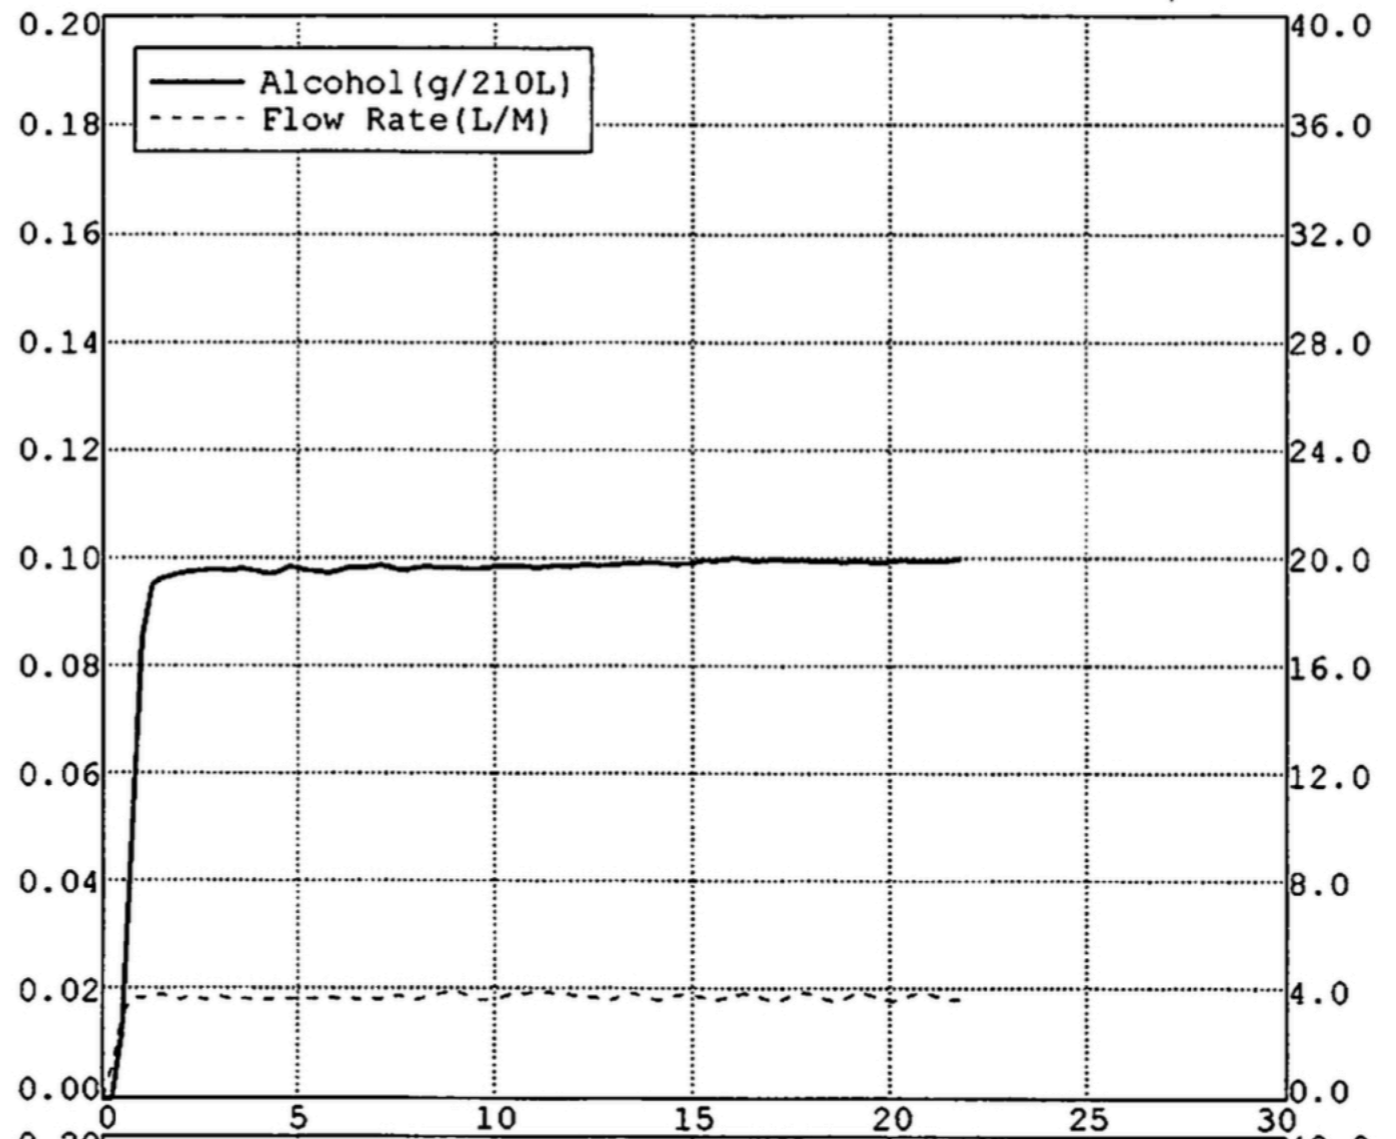

SUPERVISOR TEST

BFO

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 141906

Date: 04/12/2023

OPERATOR NAME:
KRISTY N ALLEN
Permit #: 49726
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 23030

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:58
INTERNAL STANDARD	VERIFIED	05:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	05:58
BLANK TEST	0.00	05:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	06:00
BLANK TEST	0.00	06:01
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	06:01
BLANK TEST	0.00	06:02

