

SUPERVISOR TEST

CEO




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 07/29/2021

OPERATOR NAME:
ZACHARY S PRZYBYLA
Permit #: 49339
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:47
INTERNAL STANDARD	VERIFIED	03:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:48
BLANK TEST	0.00	03:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:49
BLANK TEST	0.00	03:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:50
BLANK TEST	0.00	03:51

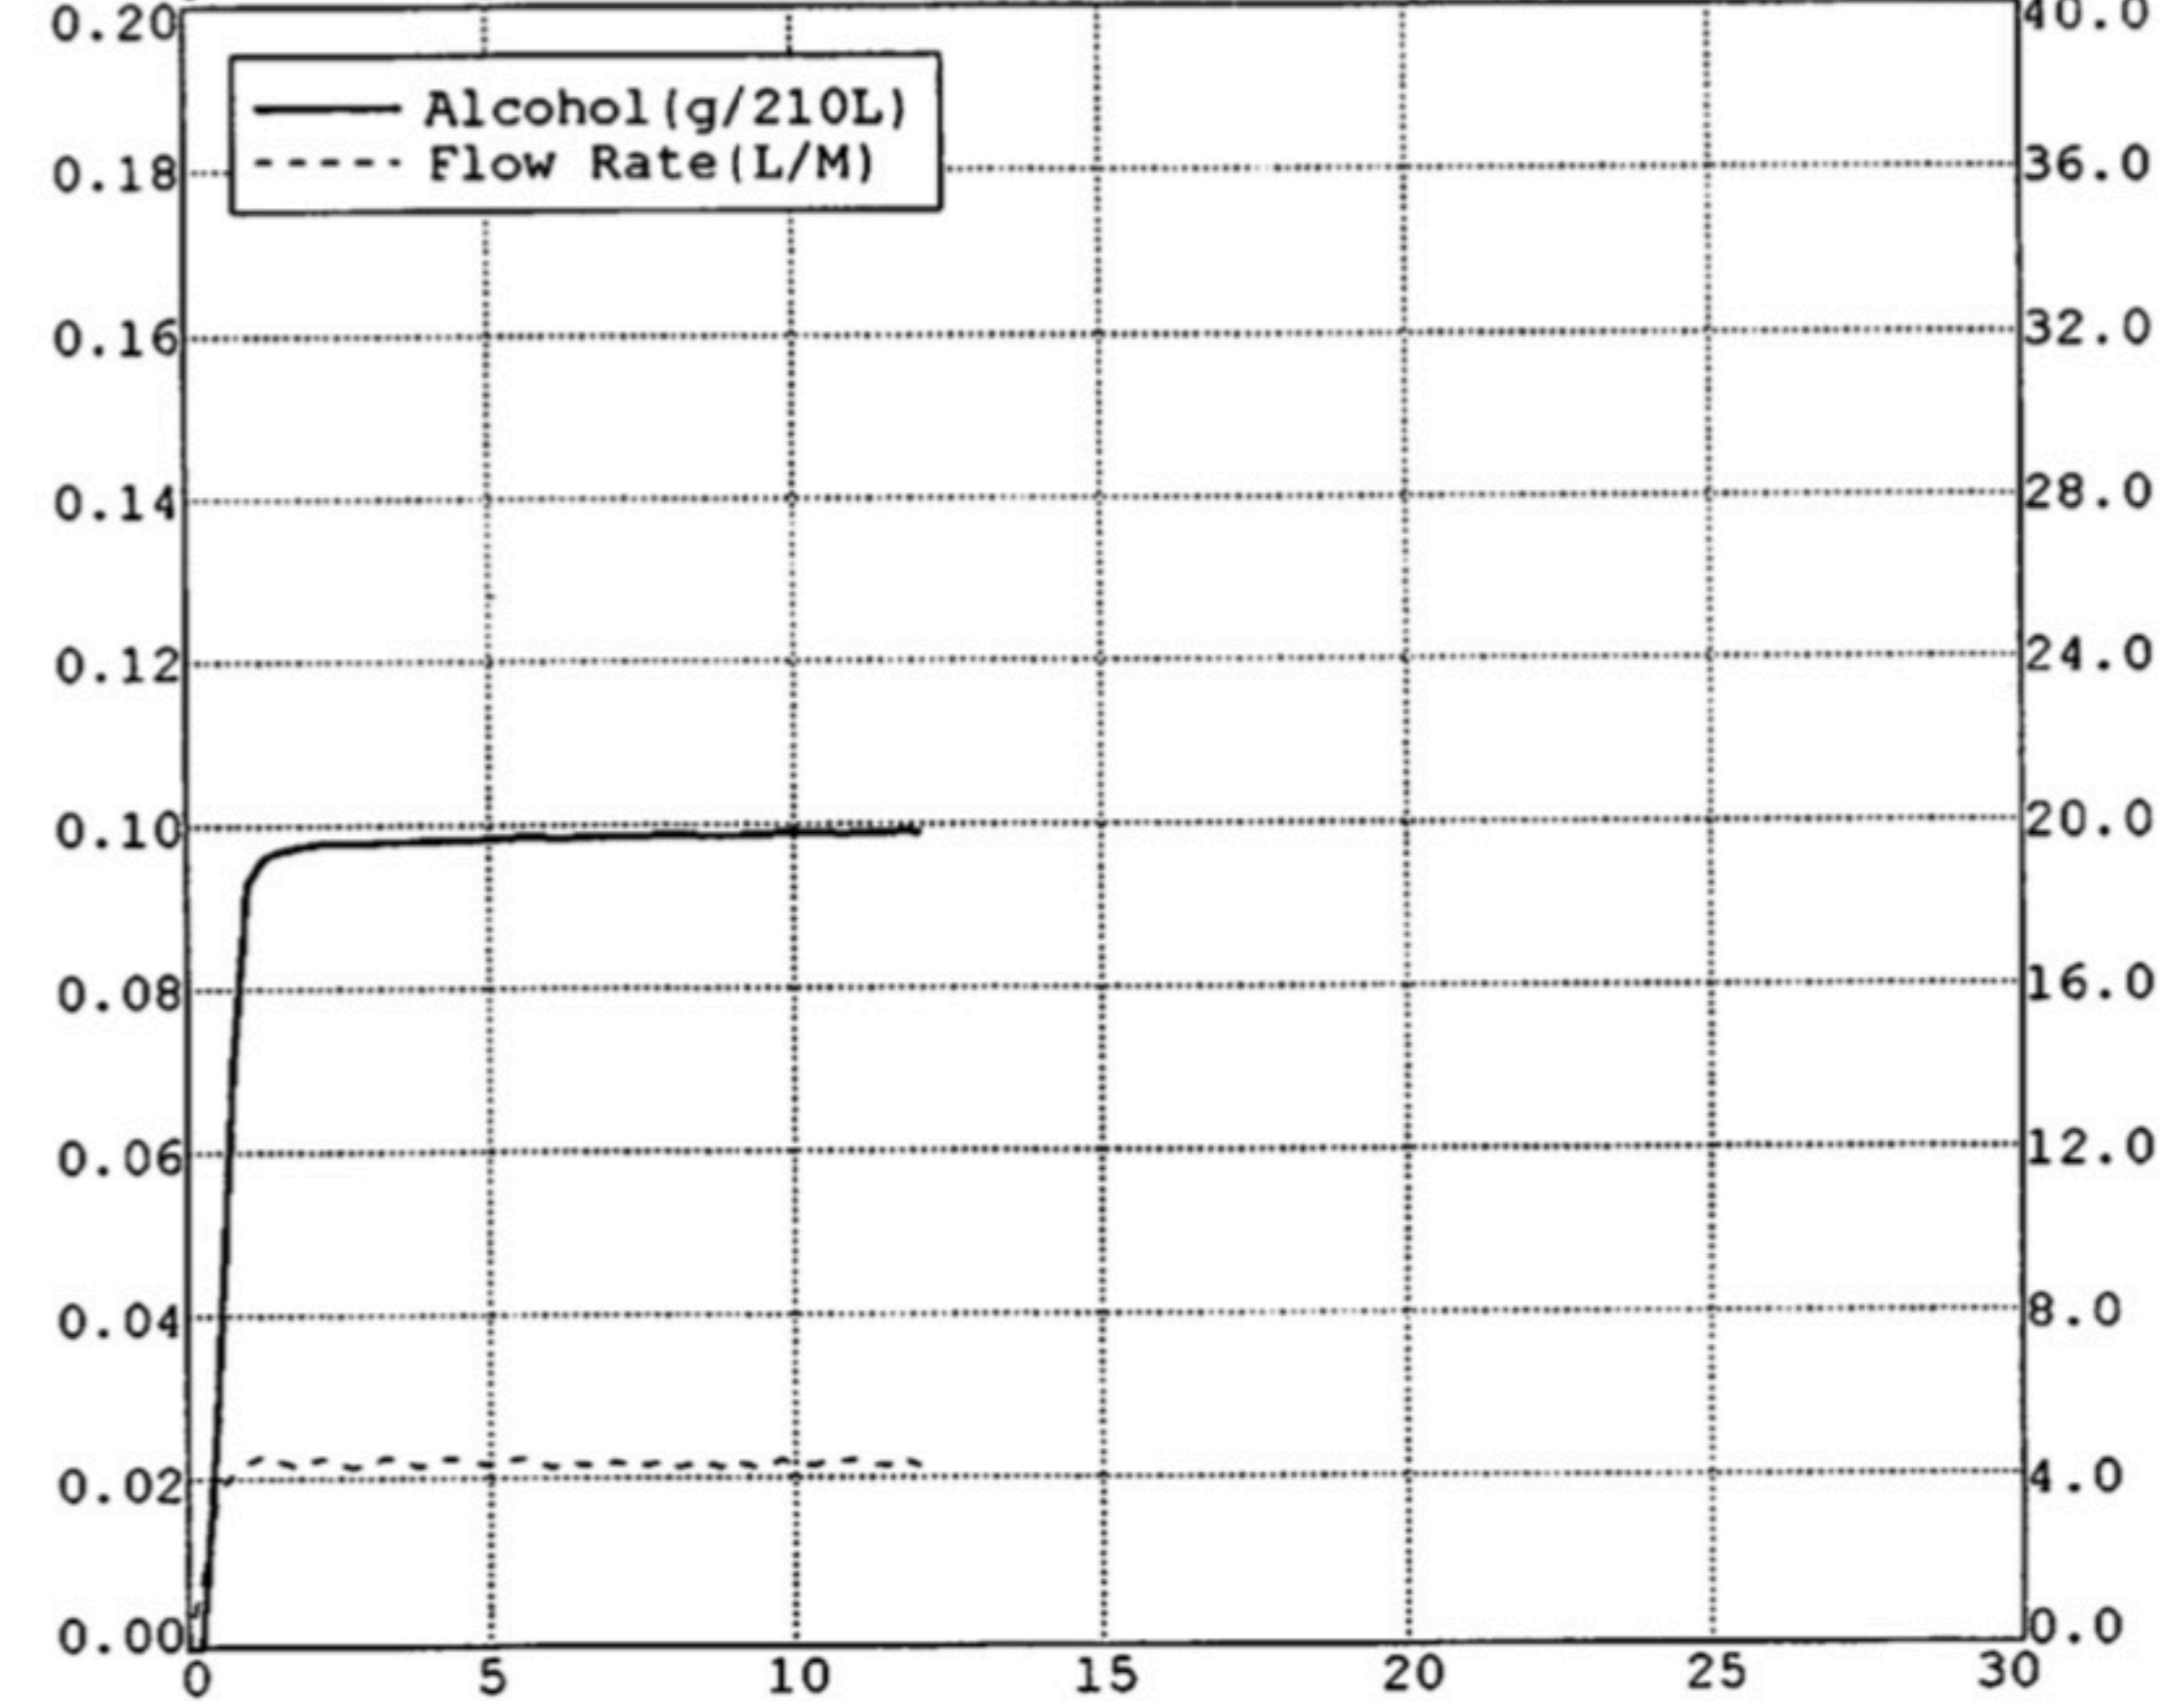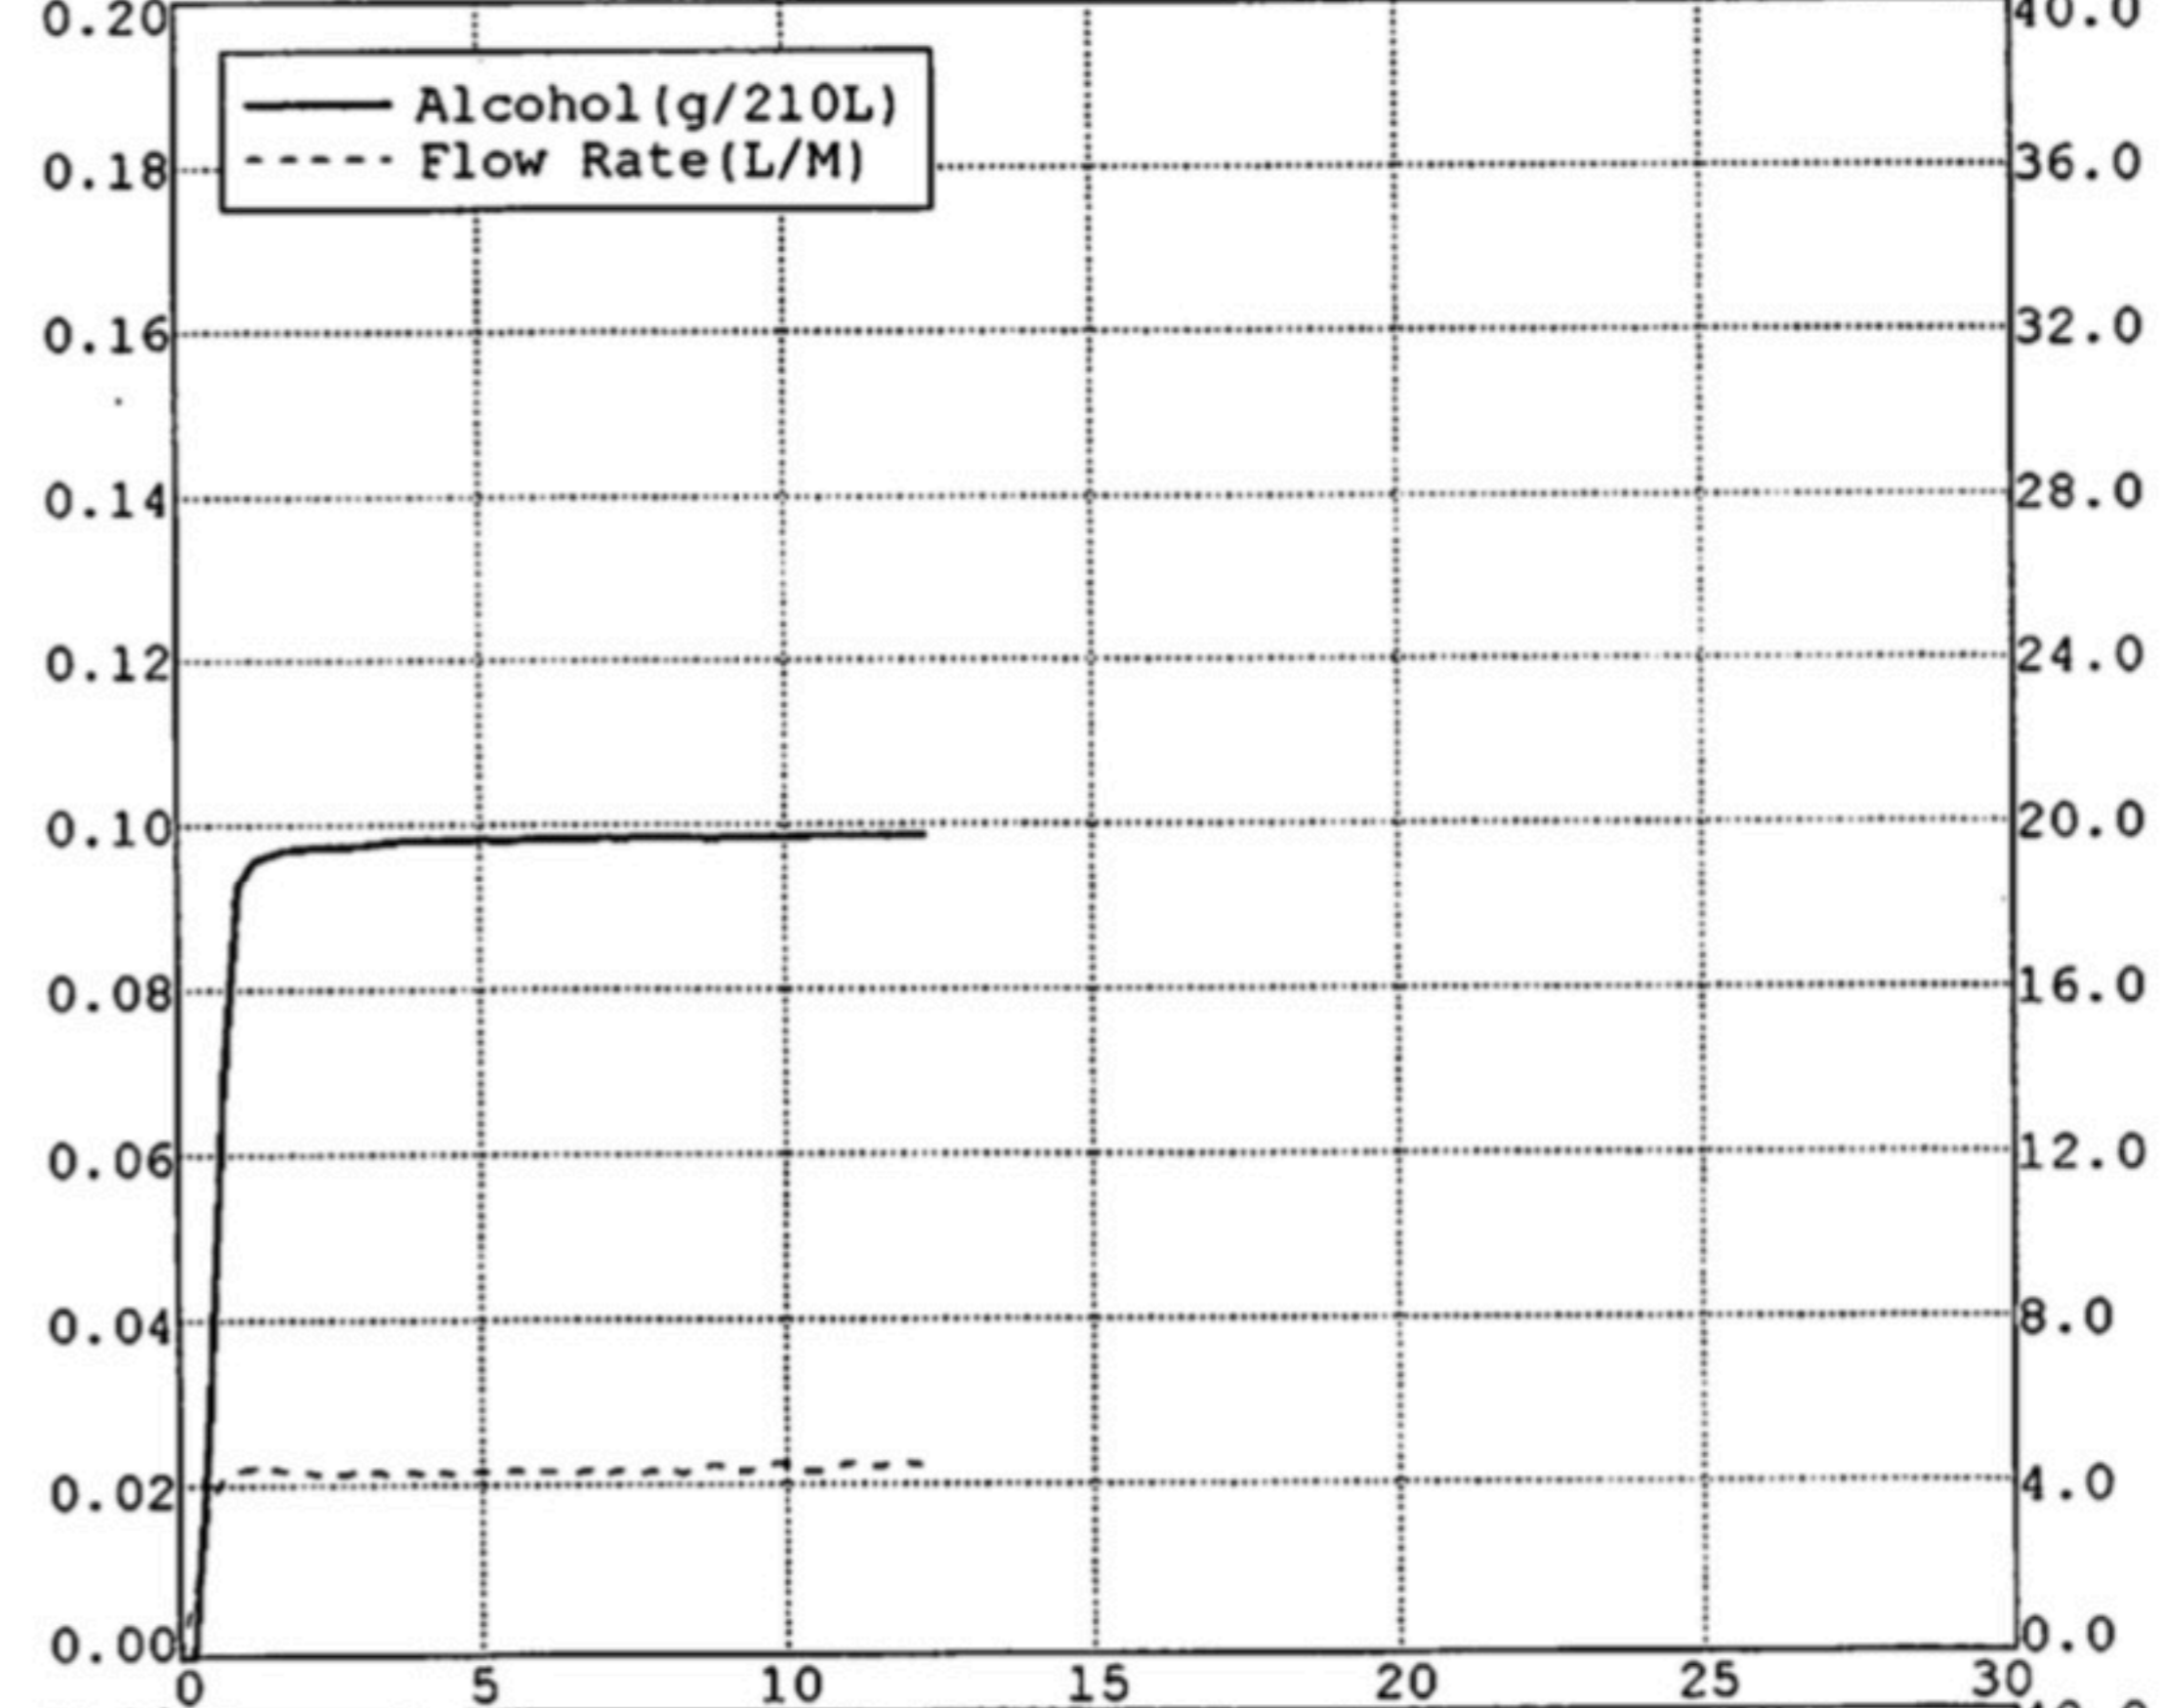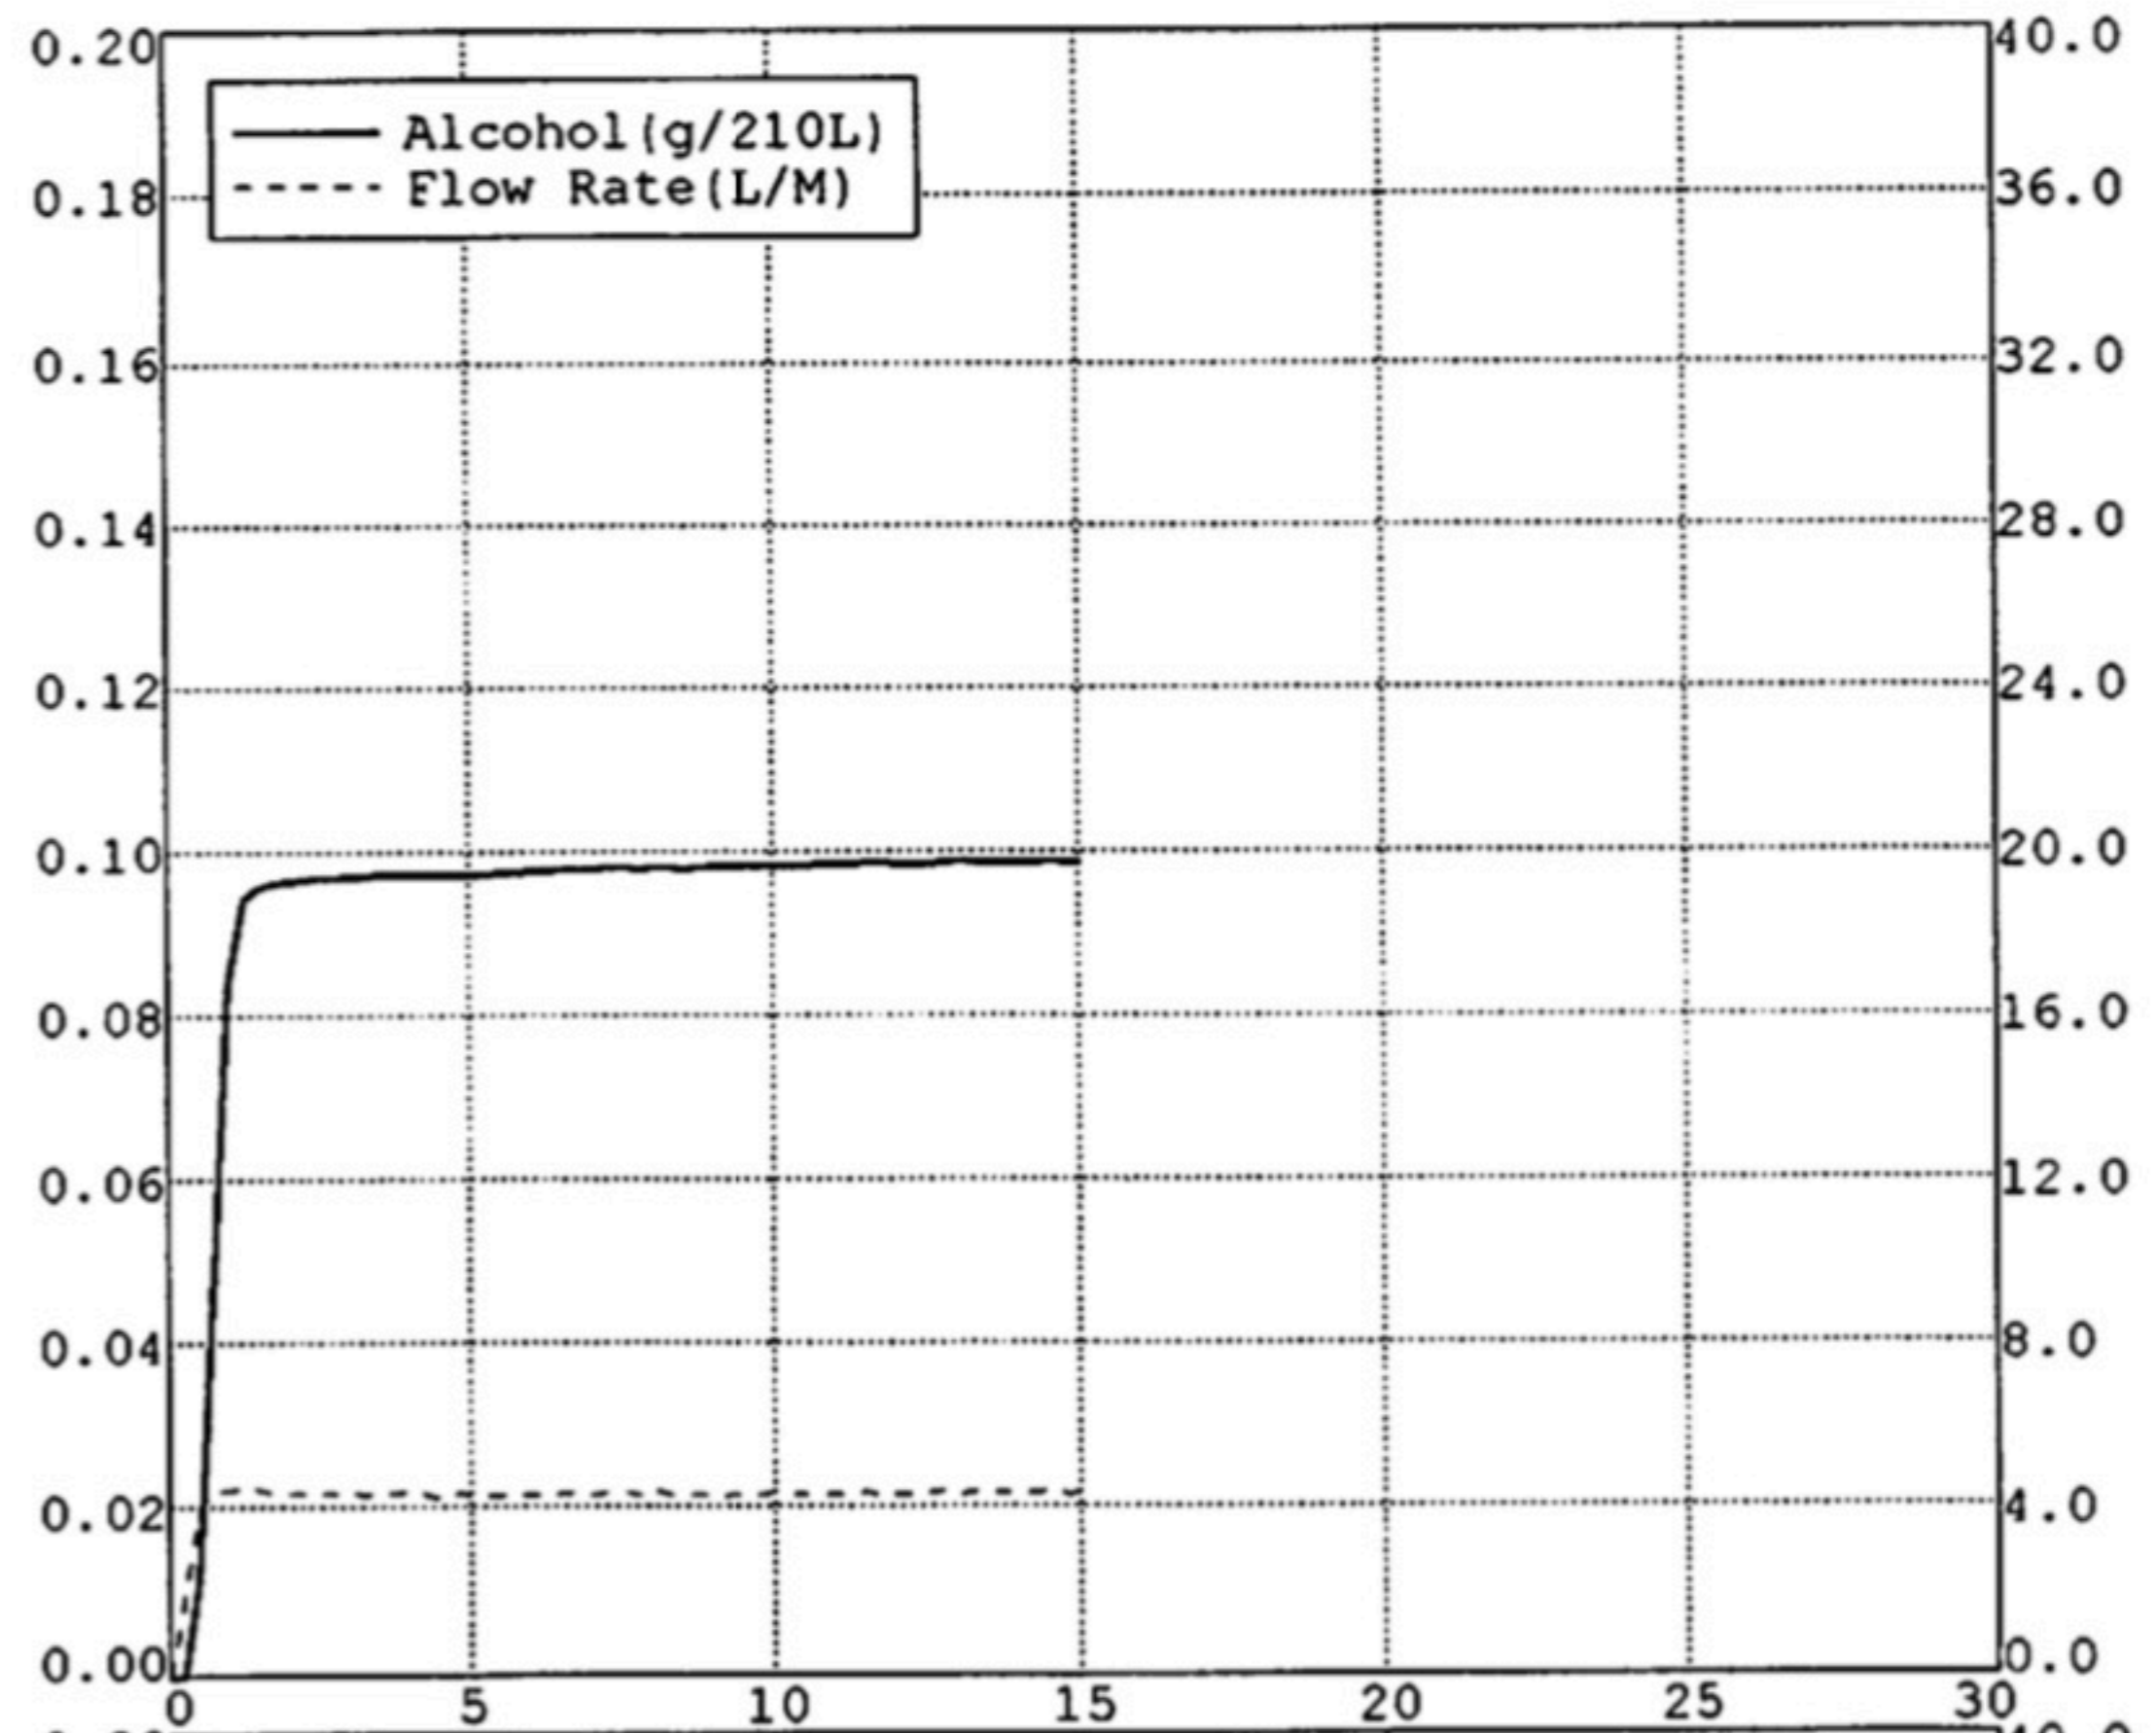

SUPERVISOR TEST



ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 08/05/2021

OPERATOR NAME:
STEVEN P EILERS
Permit #: 49321
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:23
INTERNAL STANDARD	VERIFIED	00:23
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:24
BLANK TEST	0.00	00:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:25
BLANK TEST	0.00	00:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:26
BLANK TEST	0.00	00:27

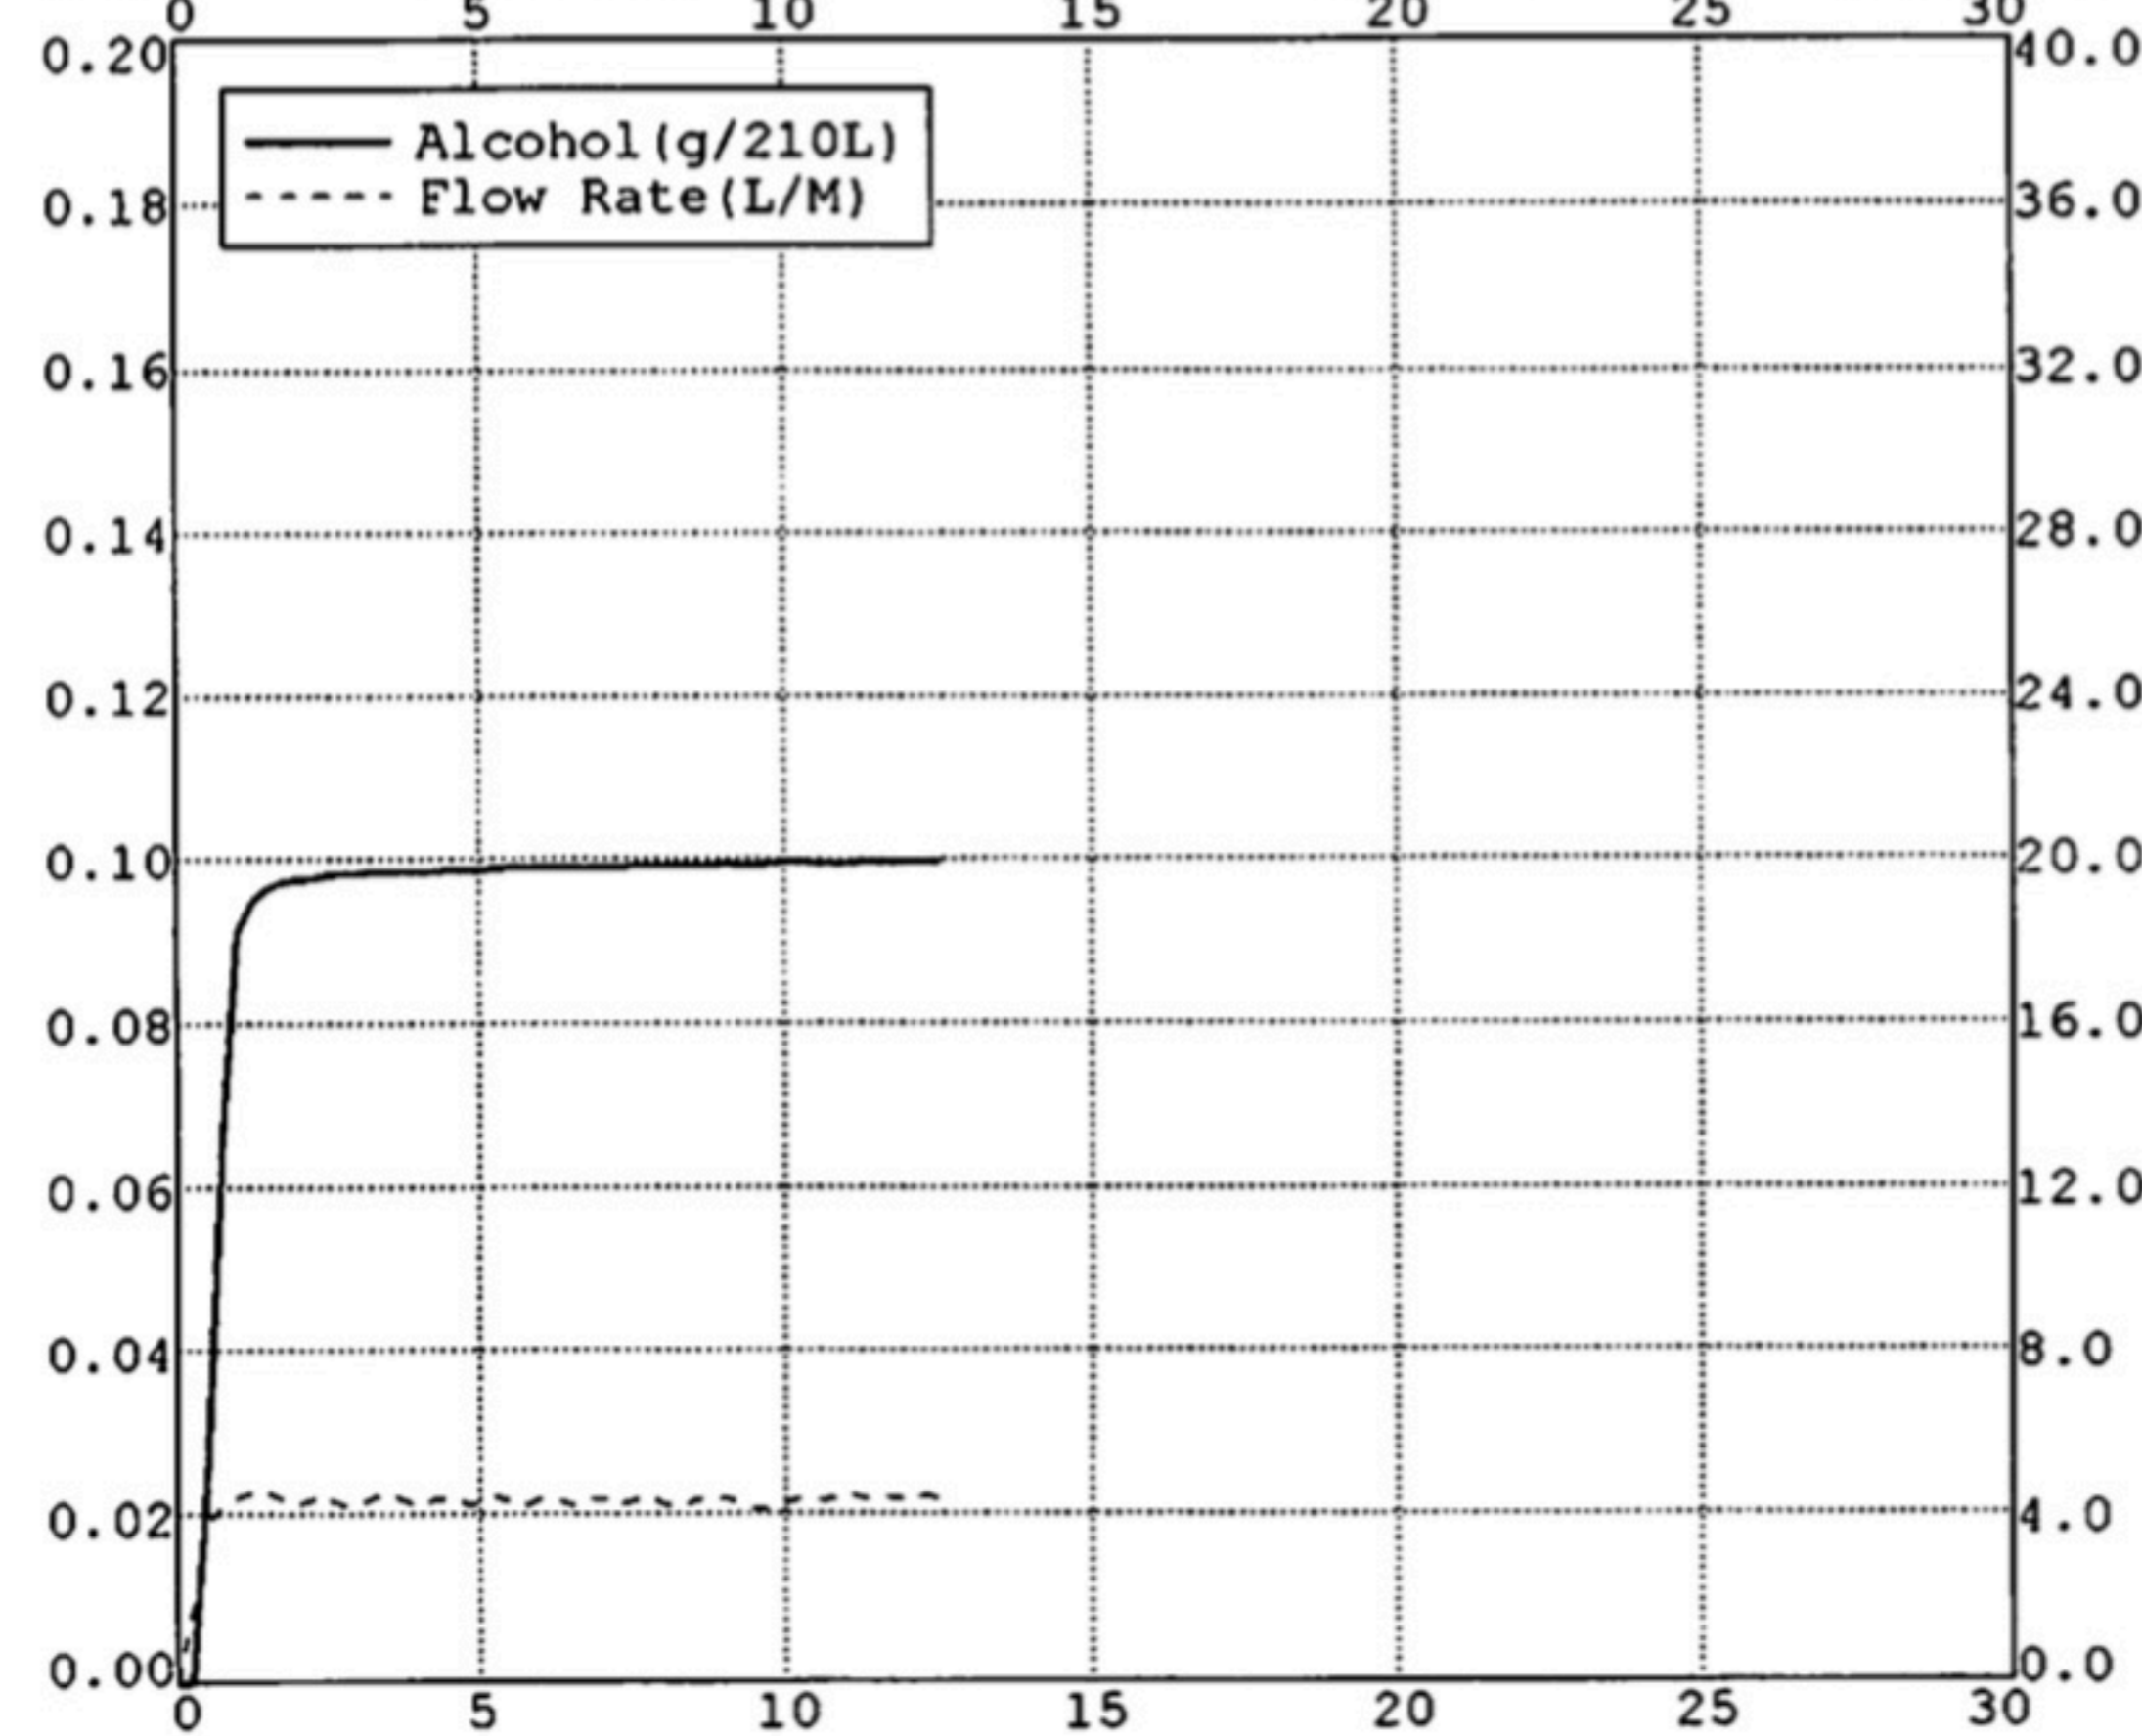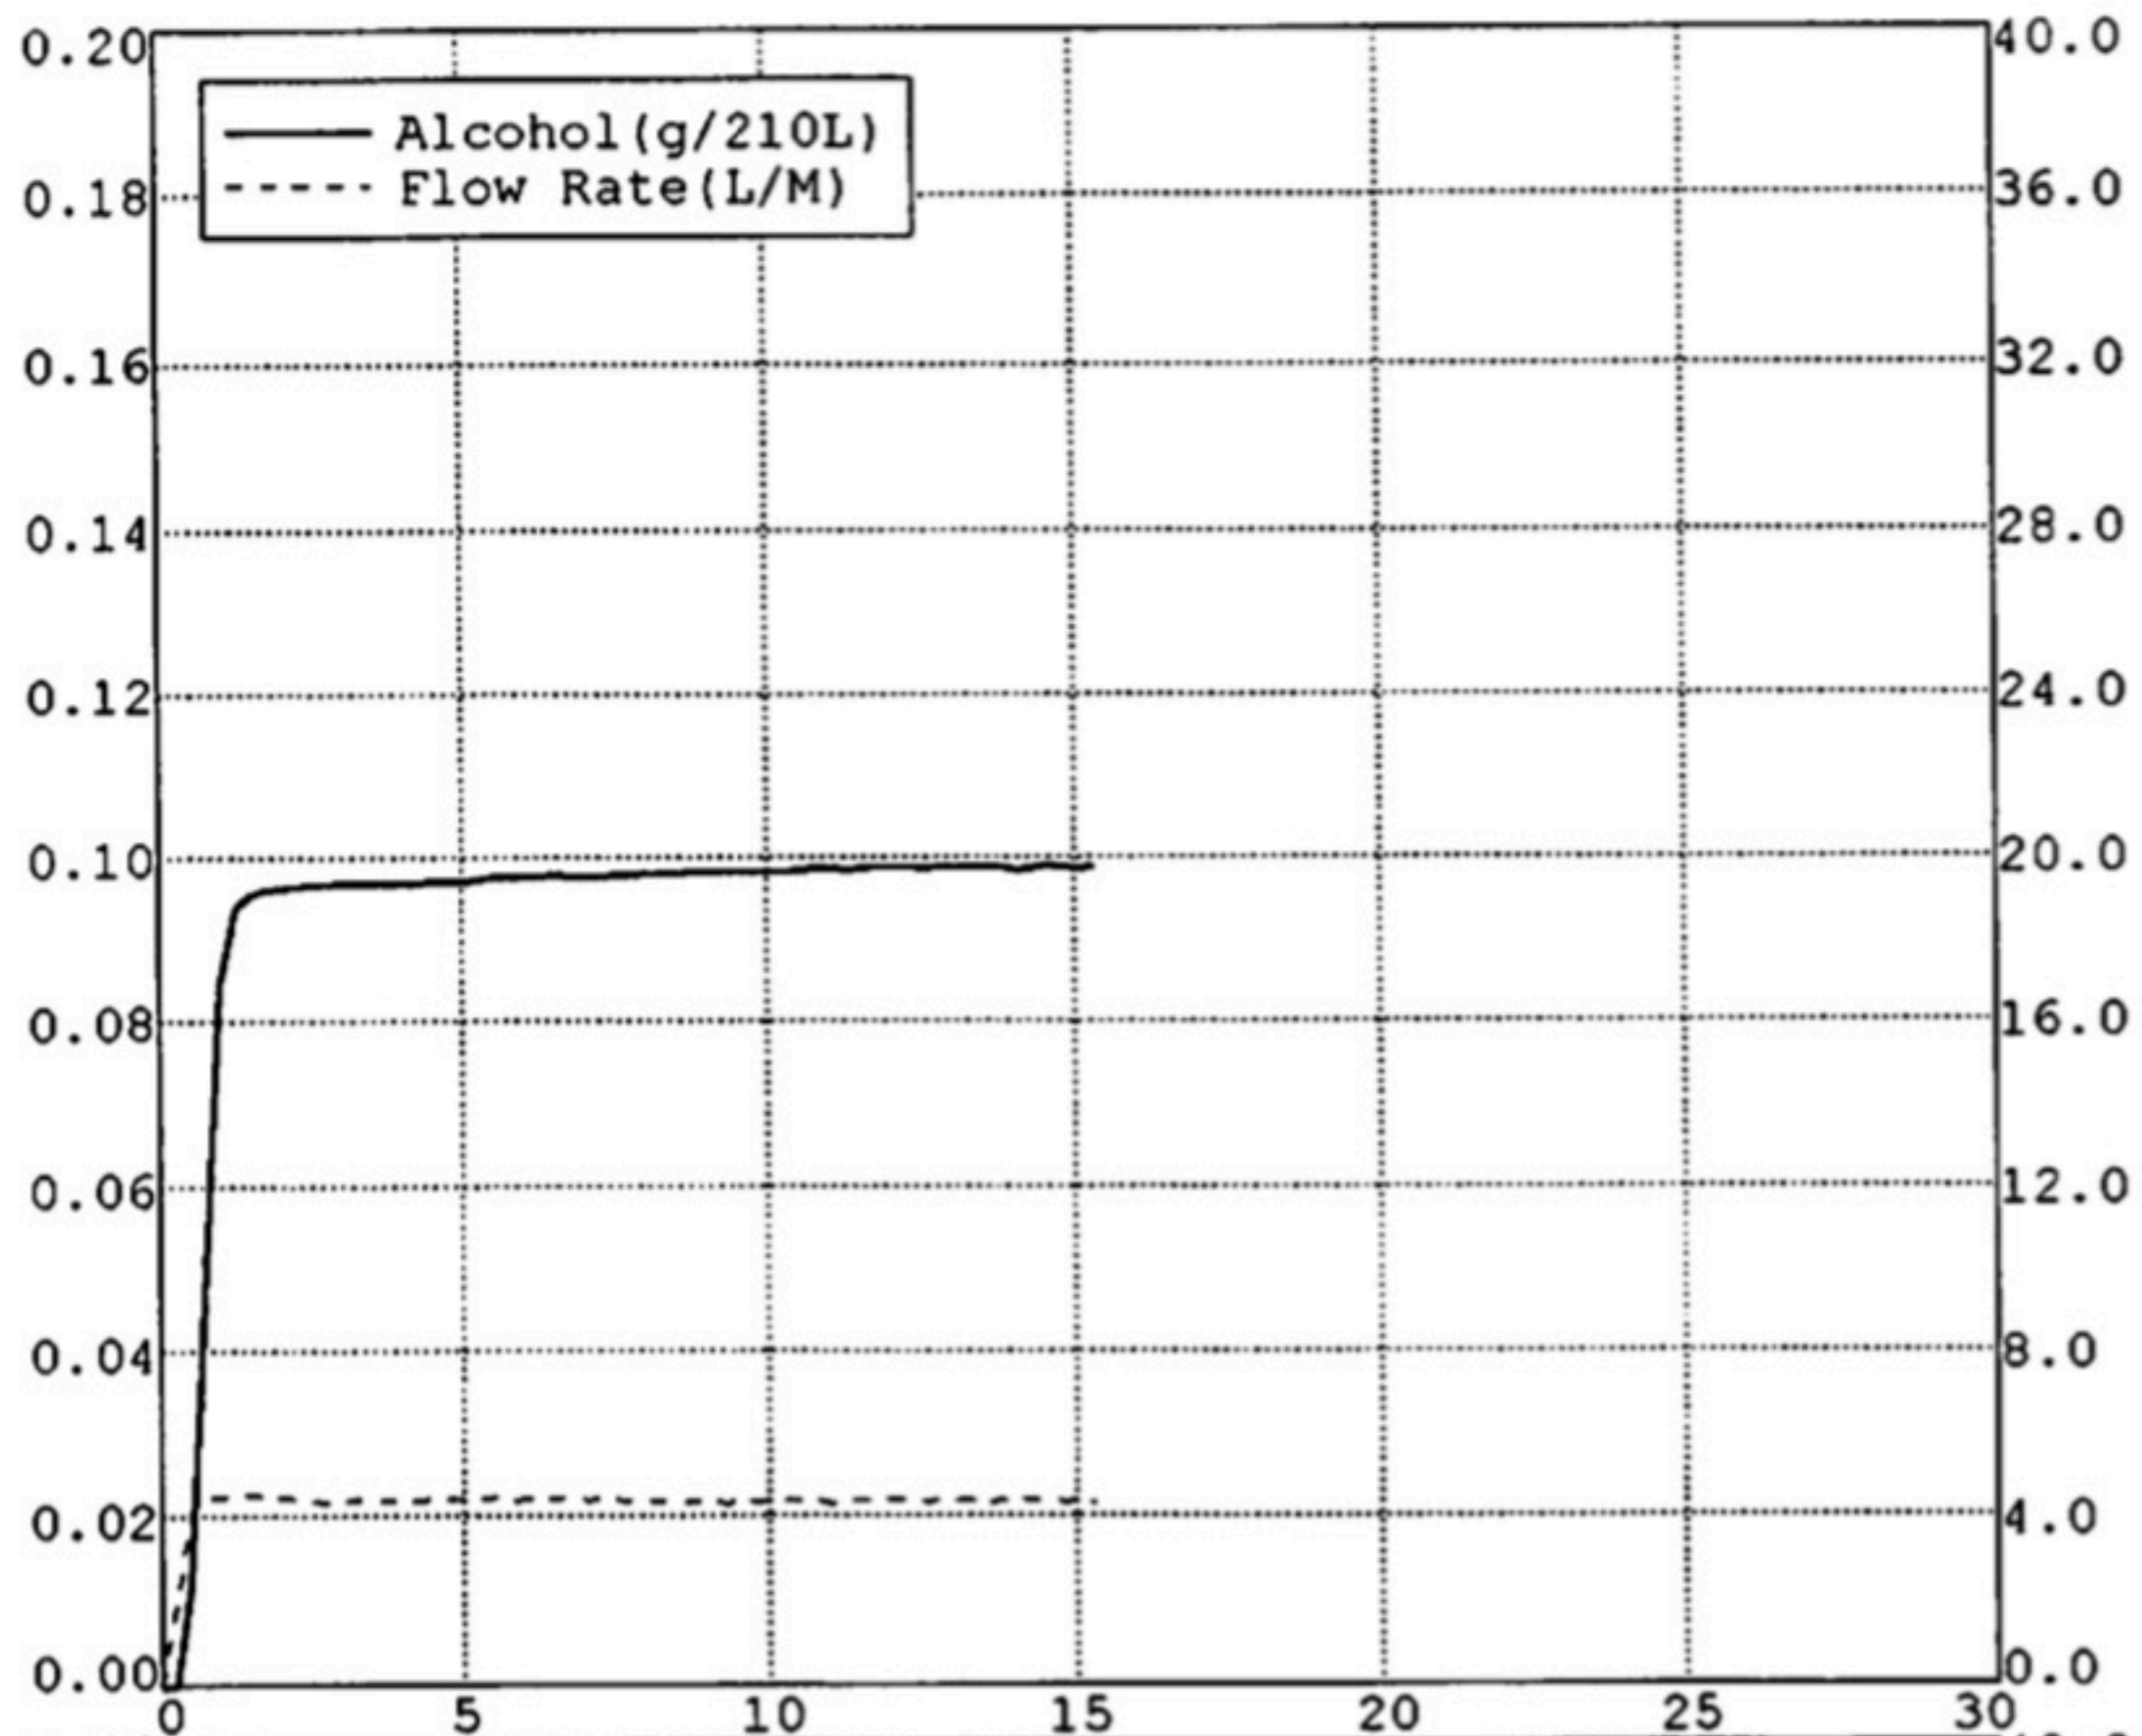

SUPERVISOR TEST

CFO

ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 08/12/2021

OPERATOR NAME:
ZACHARY S PRZYBYLA
Permit #: 49339
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 21179

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:09
INTERNAL STANDARD	VERIFIED	01:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:10
BLANK TEST	0.00	01:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:11
BLANK TEST	0.00	01:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:12
BLANK TEST	0.00	01:13

