

SUPERVISOR TEST

ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906



LFO

Date: 02/11/2026

OPERATOR NAME:
STEVEN P EILERS
Permit #: 49321
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:25
INTERNAL STANDARD	VERIFIED	23:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:26
BLANK TEST	0.00	23:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:27
BLANK TEST	0.00	23:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:28
BLANK TEST	0.00	23:29

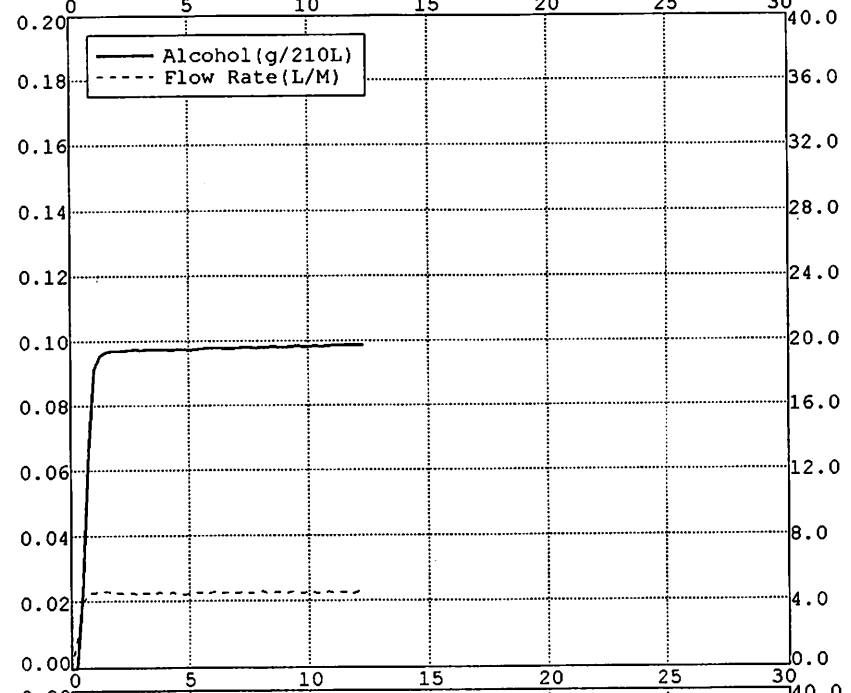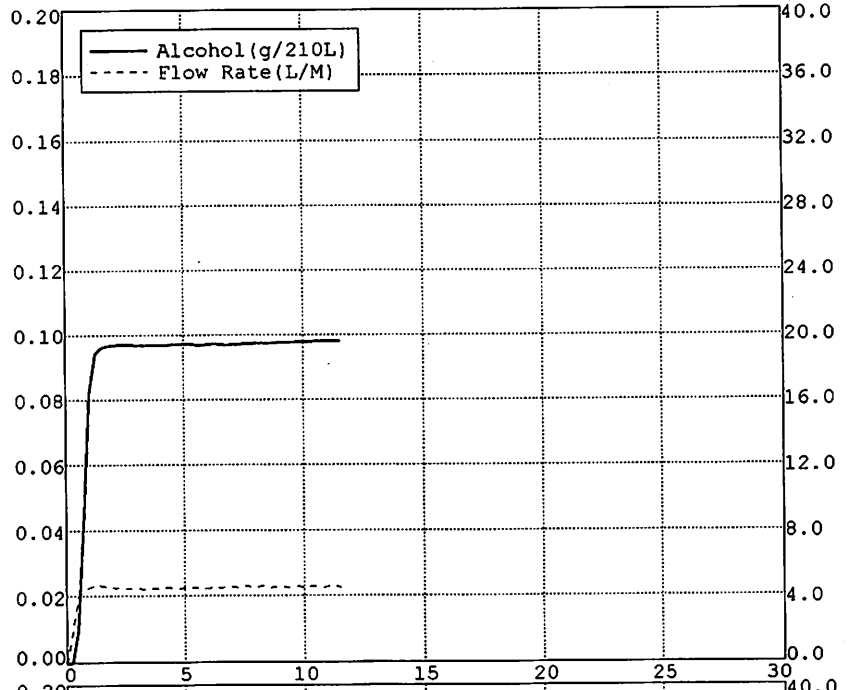

◆†Ç-▶