

SUPERVISOR TEST




ONEIDA CO.
SHERIFF'S DEPT
DATAMASTER dmt: 123906

Date: 02/04/2026

OPERATOR NAME:
BRADY A WOOD
Permit #: 52004
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:35
INTERNAL STANDARD	VERIFIED	01:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:35
BLANK TEST	0.00	01:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:37
BLANK TEST	0.00	01:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:38
BLANK TEST	0.00	01:39

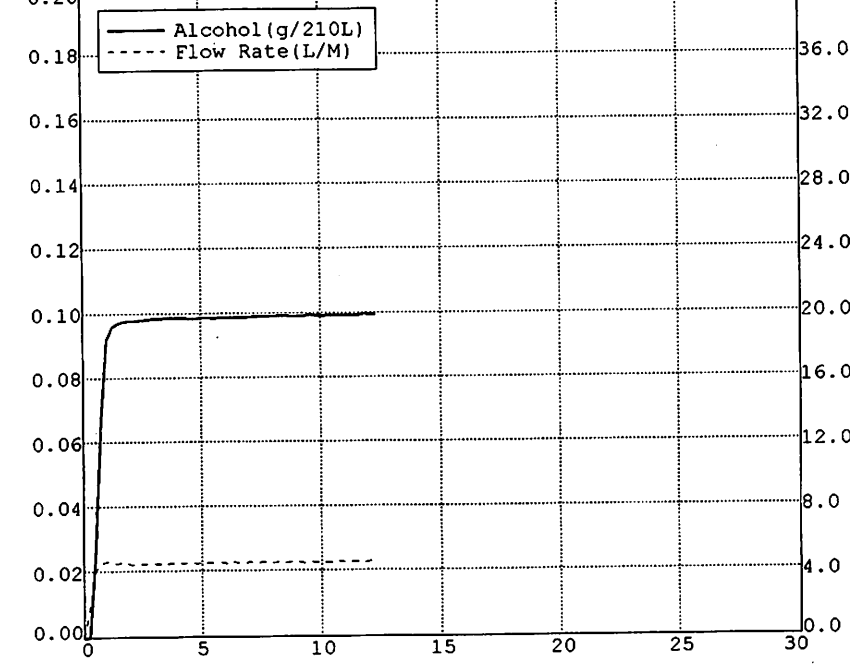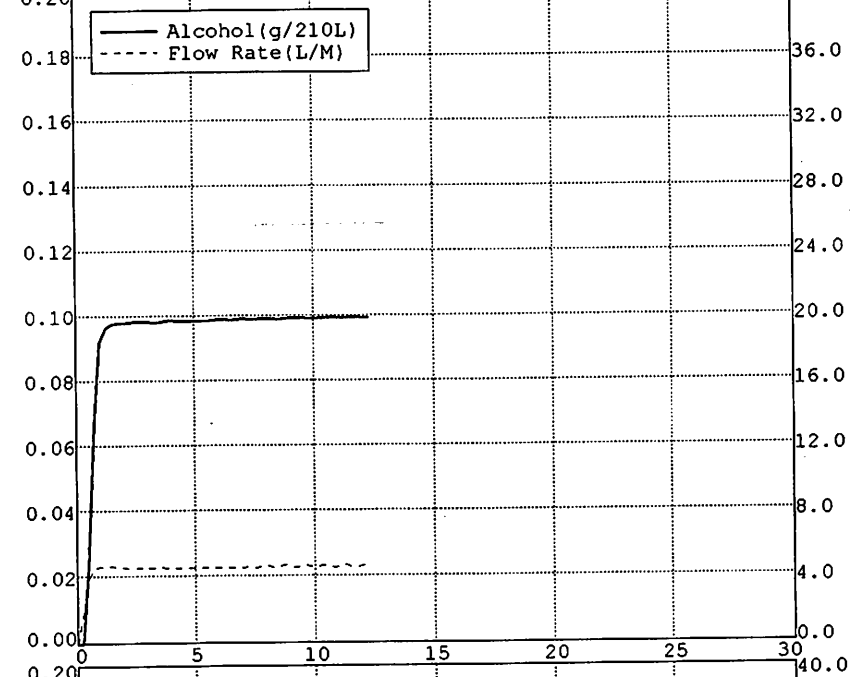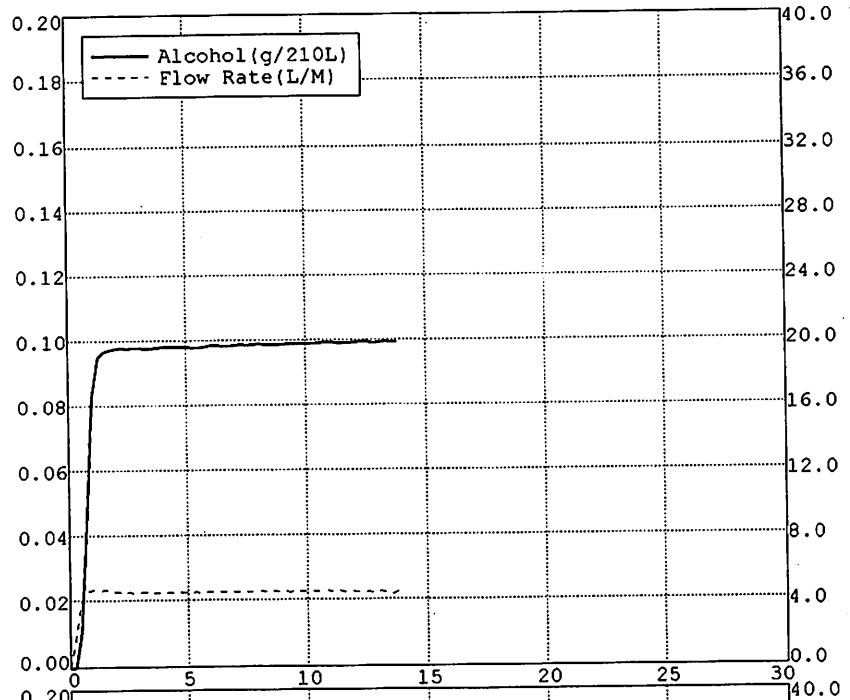

Camden Field Office

BW 66