

SUPERVISOR TEST




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 07/21/2021

OPERATOR NAME:
STEVEN P EILERS
Permit #: 49321
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:12
INTERNAL STANDARD	VERIFIED	18:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:12
BLANK TEST	0.00	18:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:13
BLANK TEST	0.00	18:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:15
BLANK TEST	0.00	18:16

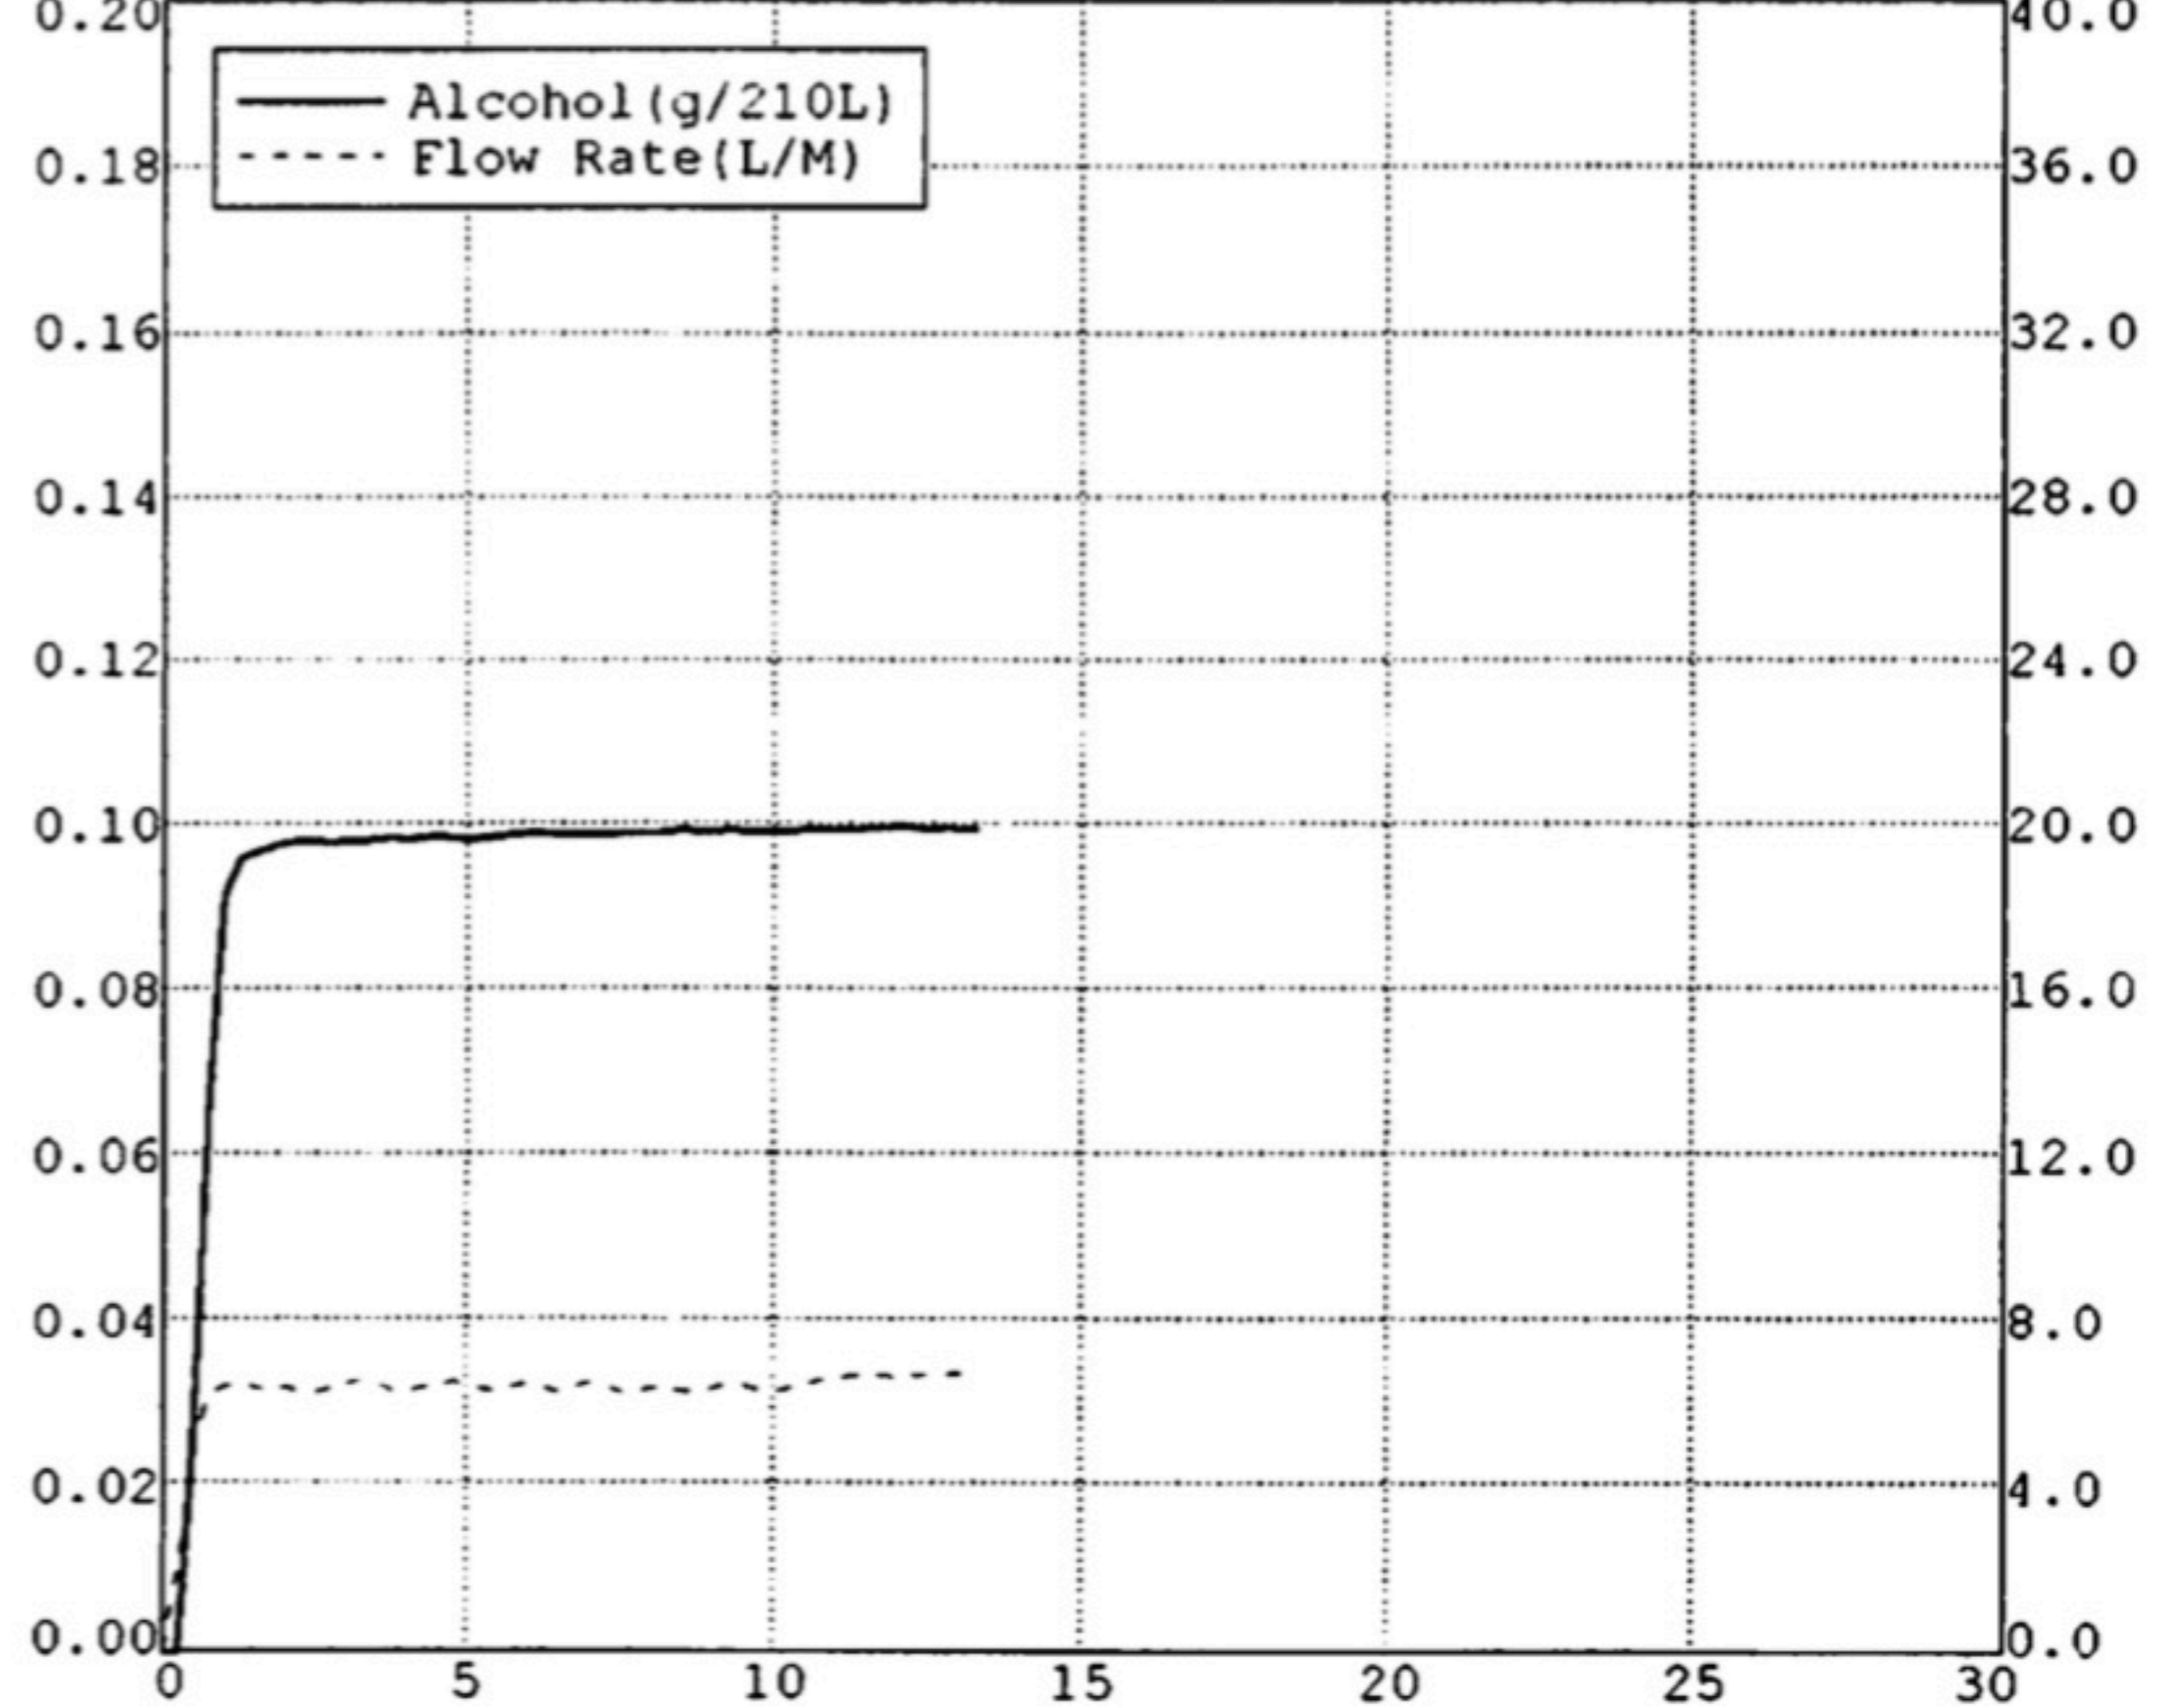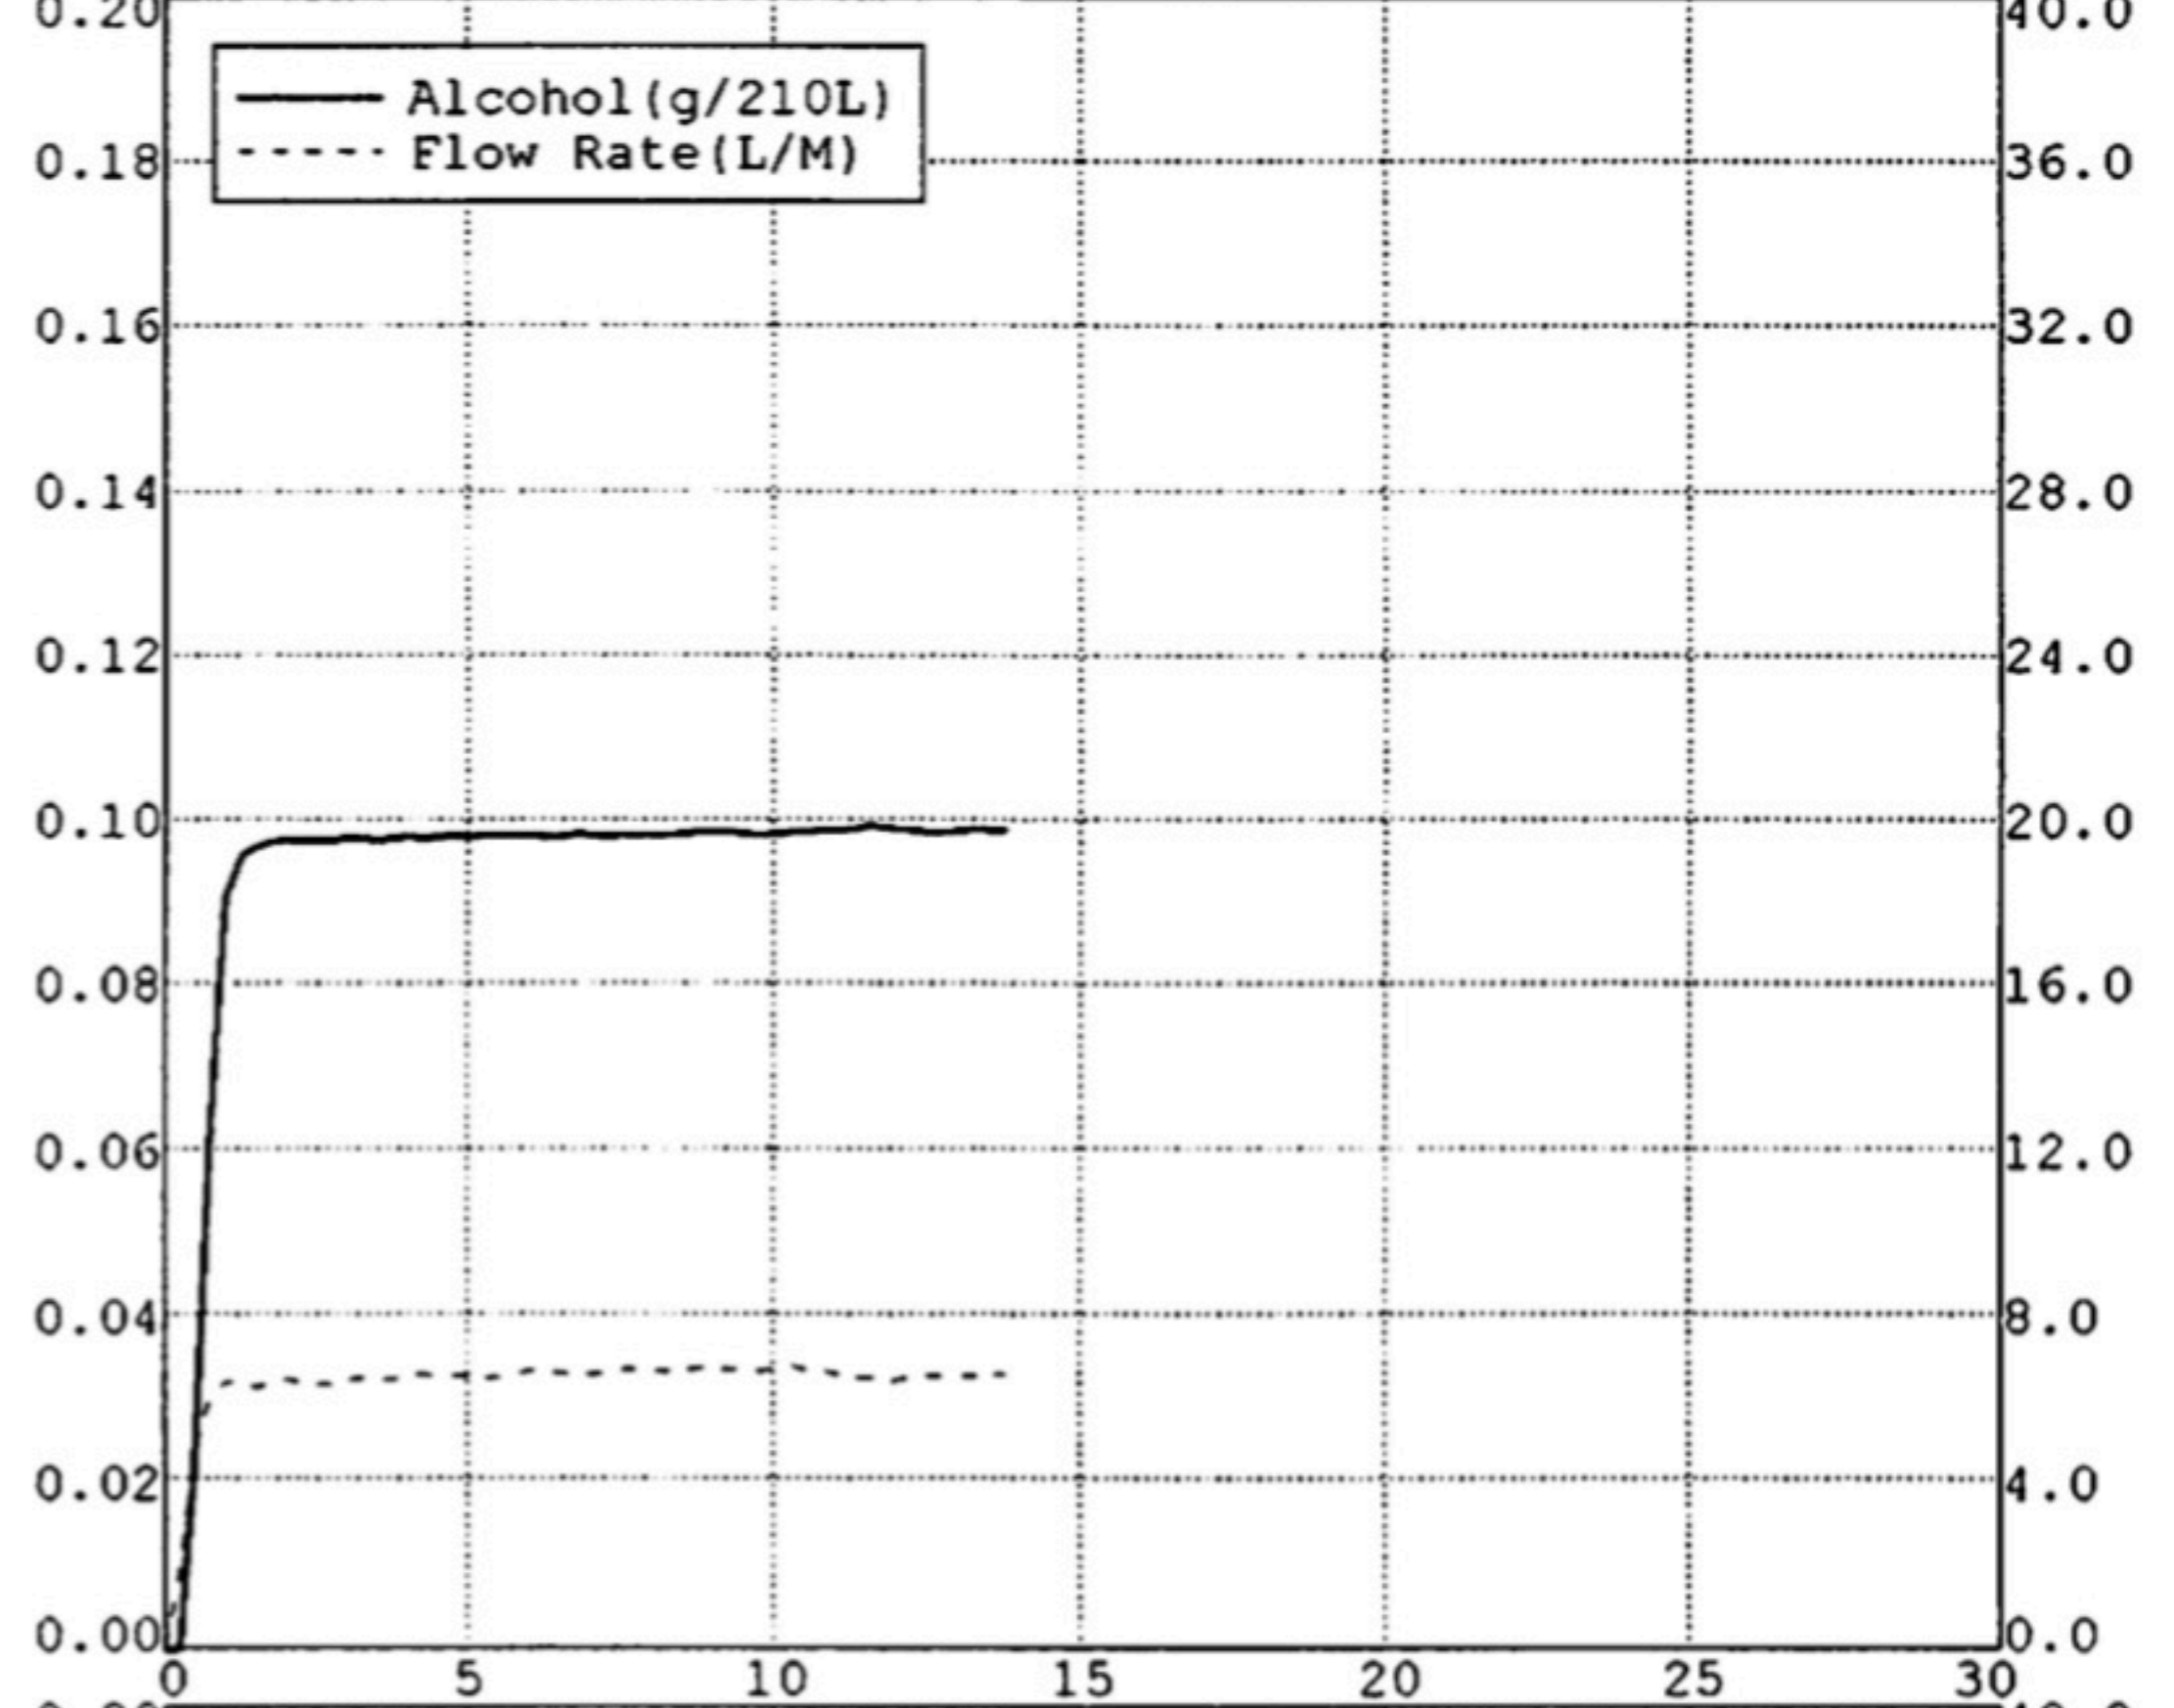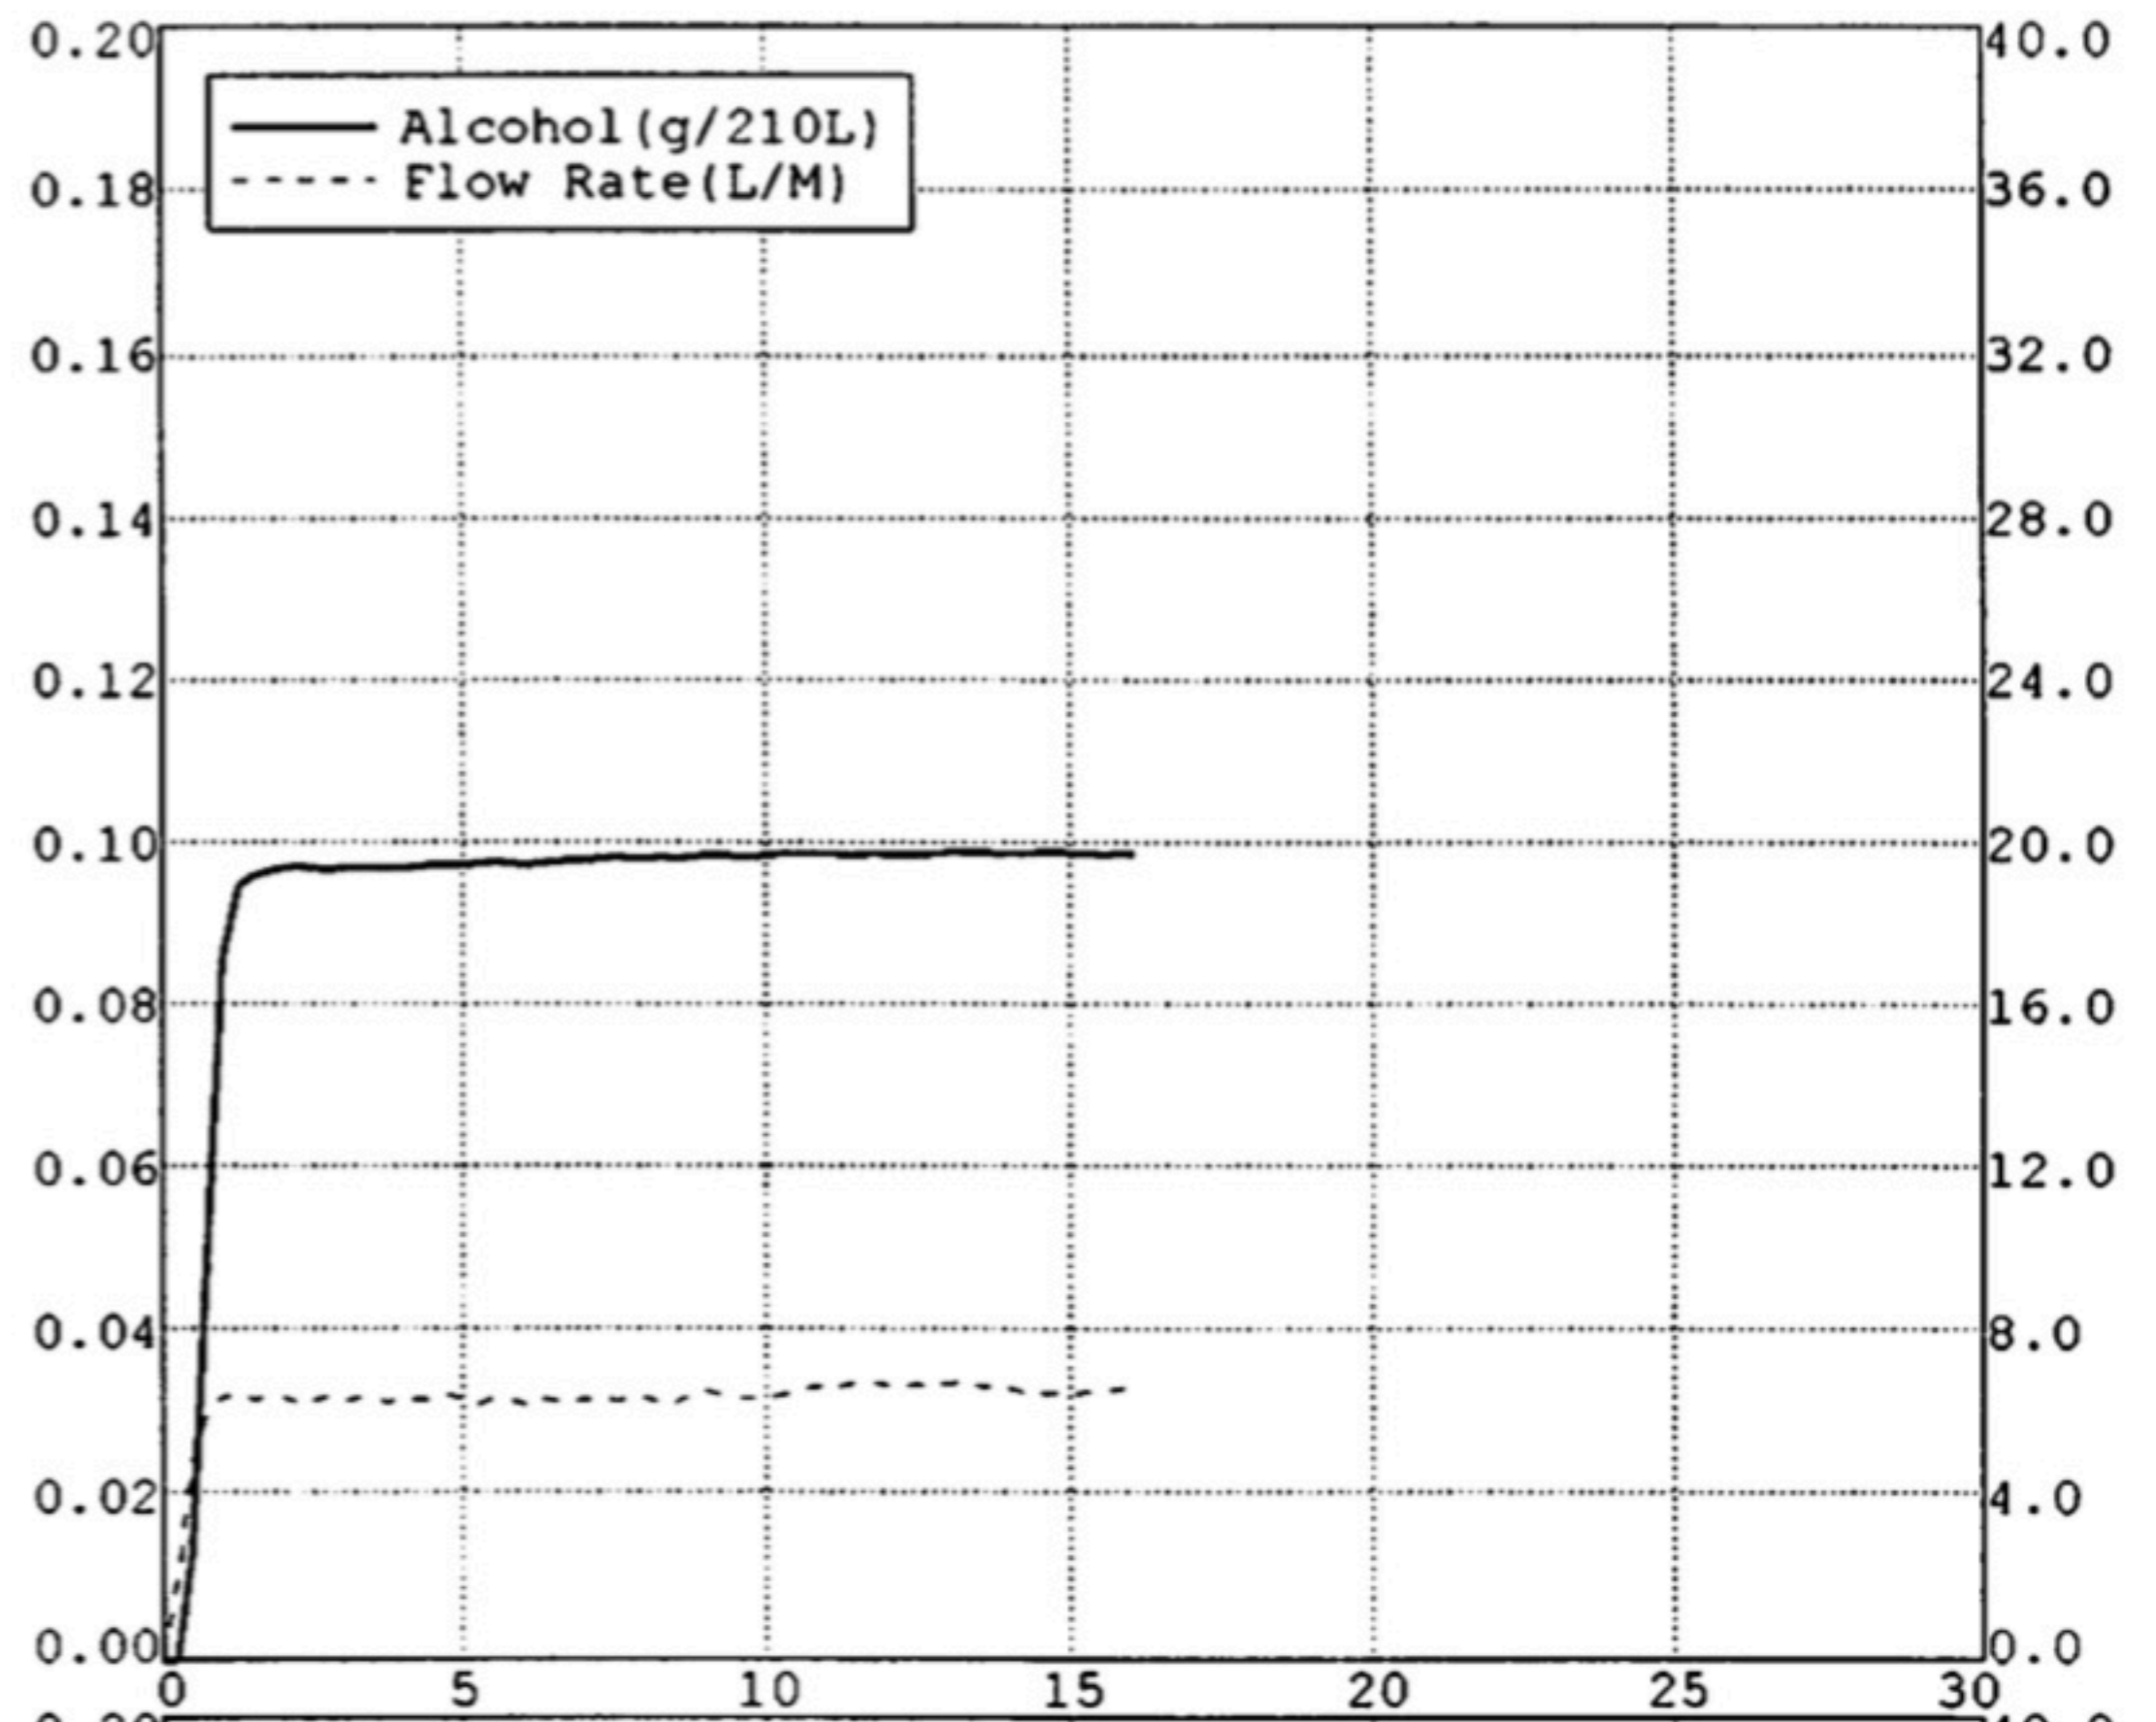

SUPERVISOR TEST

LEB

ONEIDA COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 113606

Date: 07/29/2021

OPERATOR NAME:
 BRETT A GRABELDINGER
 Permit #: 46896
 Operator Agency/Dept: ONEIDA CO. SO
 Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:51
INTERNAL STANDARD	VERIFIED	01:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:52
BLANK TEST	0.00	01:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:53
BLANK TEST	0.00	01:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:54
BLANK TEST	0.00	01:55

