

SOLUTION CHANGE




ONEIDA COUNTY  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 113606

Date: 10/01/2022

OPERATOR NAME:  
 NOAH A DANQUER  
 Permit #: 50812  
 Operator Agency/Dept: ONEIDA CO. SO  
 Reference Standard #: 22260

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:15
INTERNAL STANDARD	VERIFIED	03:15
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	03:16
BLANK TEST	0.00	03:16
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	03:17
BLANK TEST	0.00	03:18
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	03:18
BLANK TEST	0.00	03:19

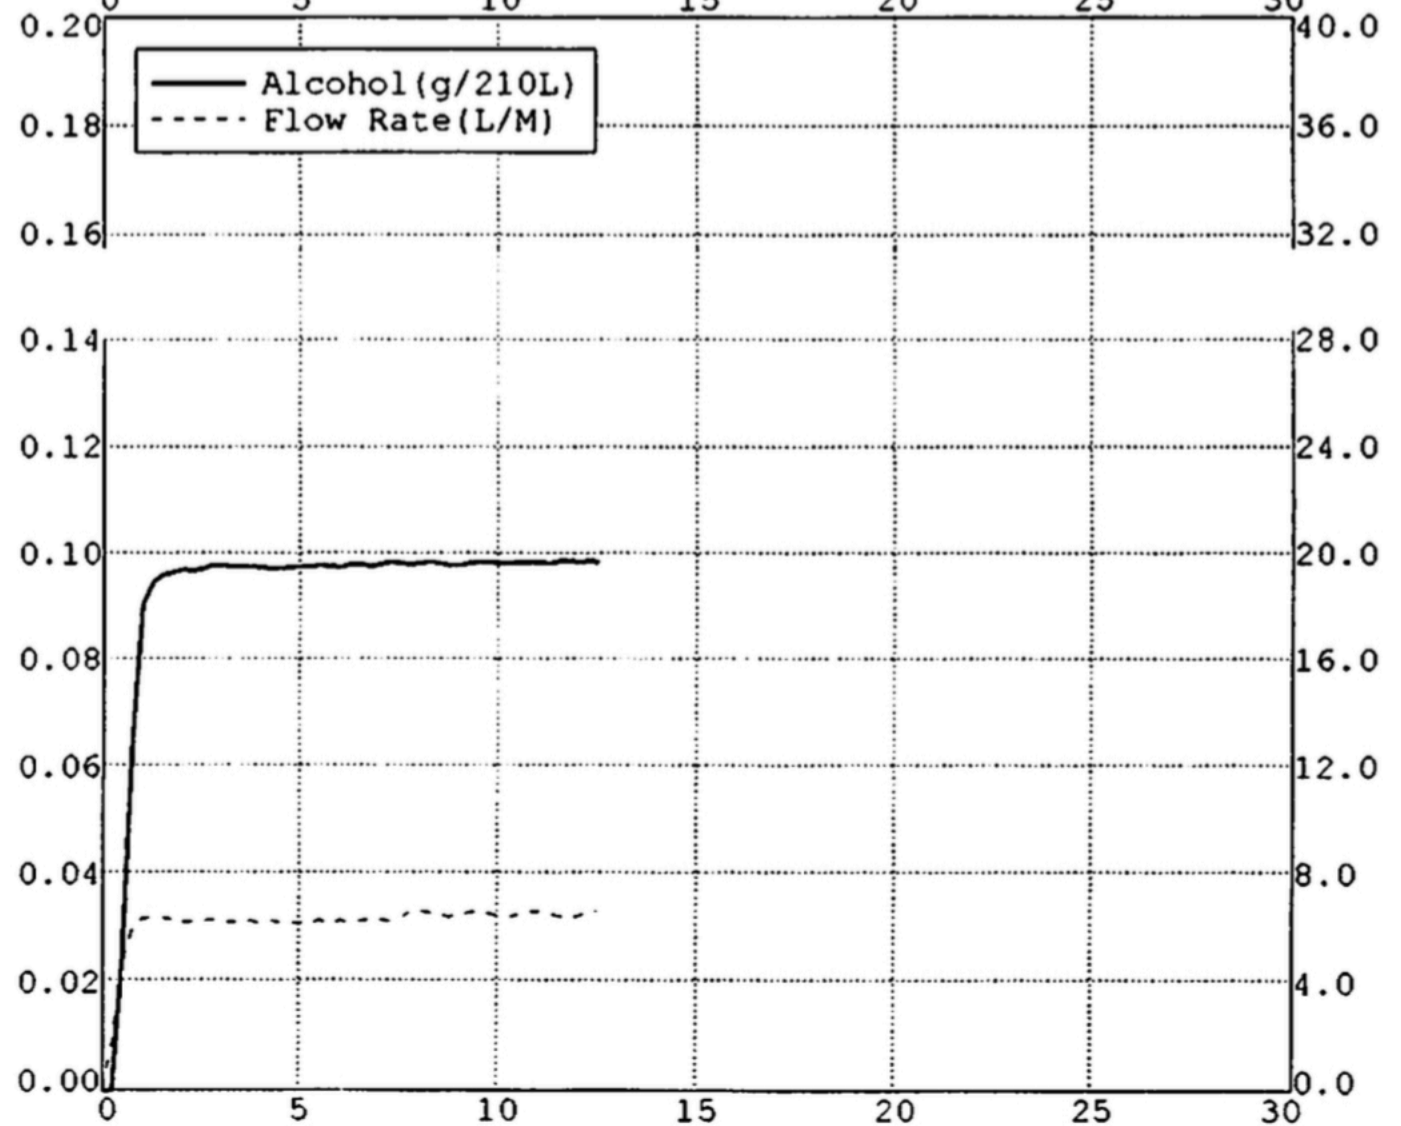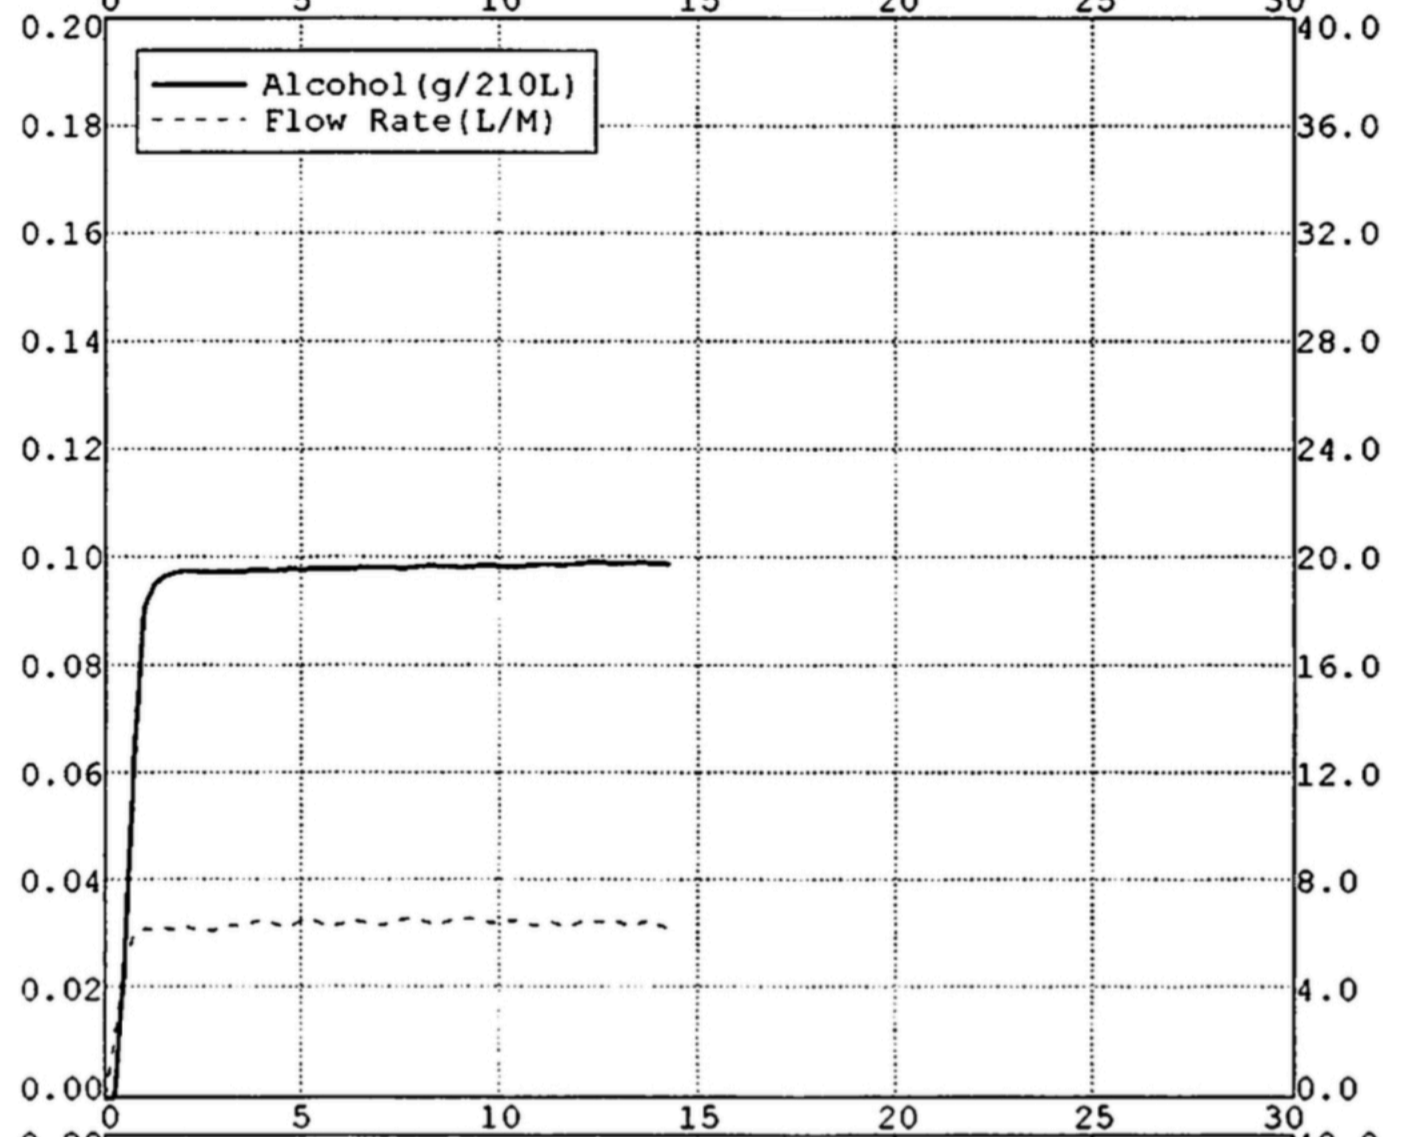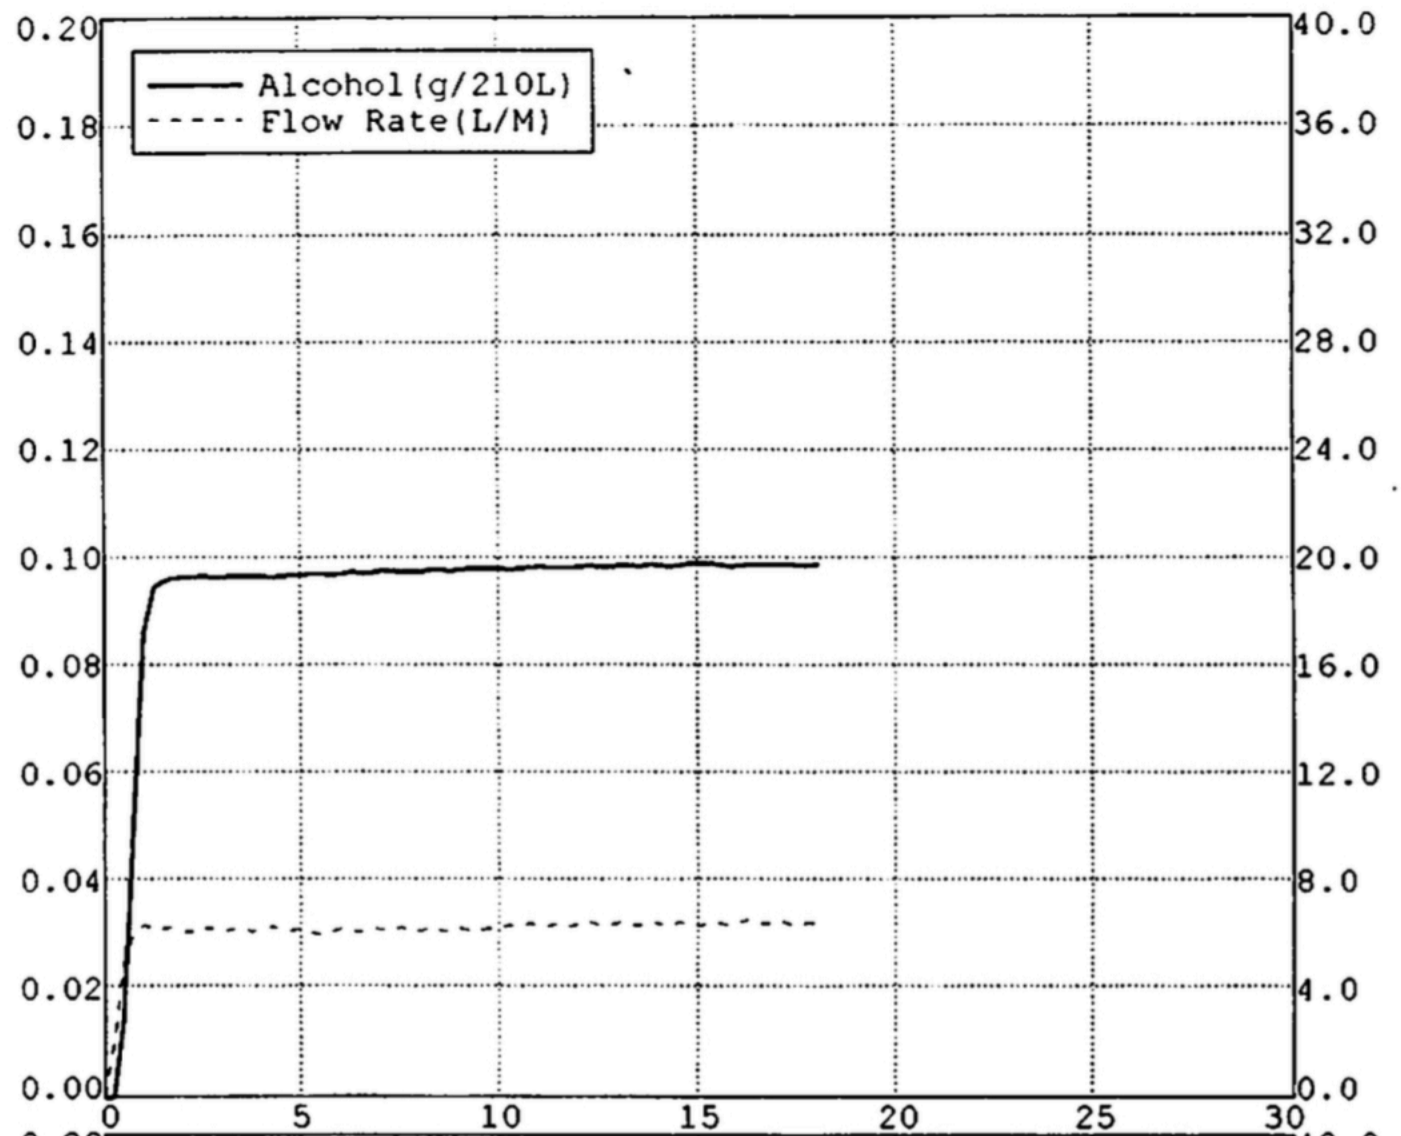

\*b0W