

SUPERVISOR TEST




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 09/28/2022

OPERATOR NAME:
NOAH A DANQUER
Permit #: 50812
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:02
INTERNAL STANDARD	VERIFIED	06:02
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	06:02
BLANK TEST	0.00	06:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	06:03
BLANK TEST	0.00	06:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	06:05
BLANK TEST	0.00	06:06

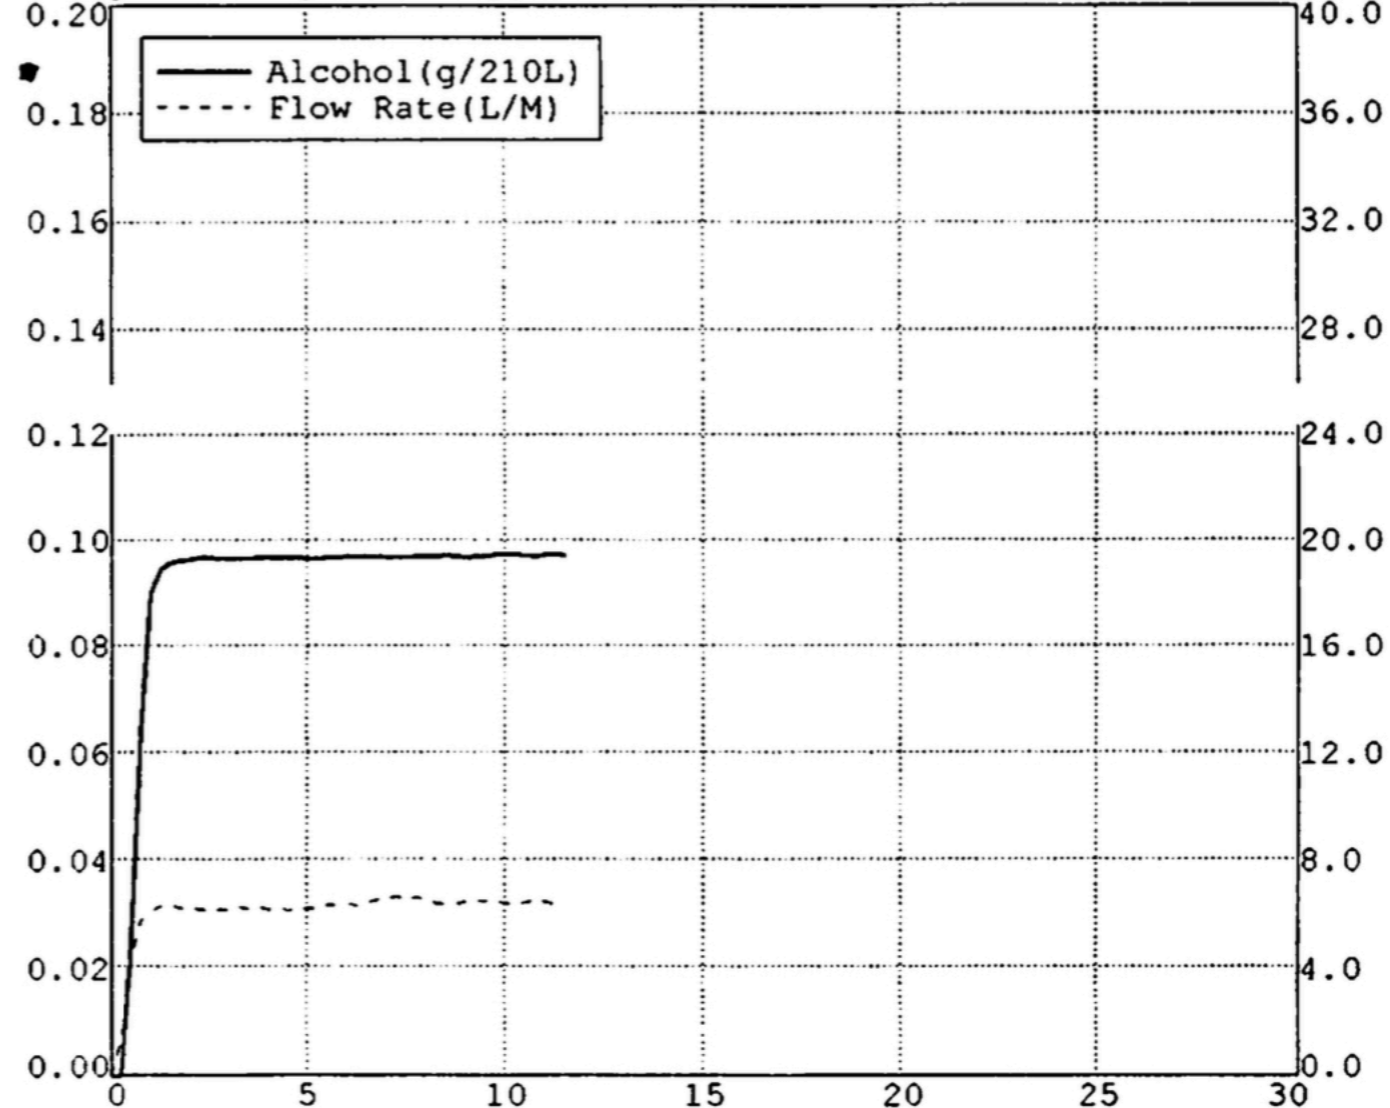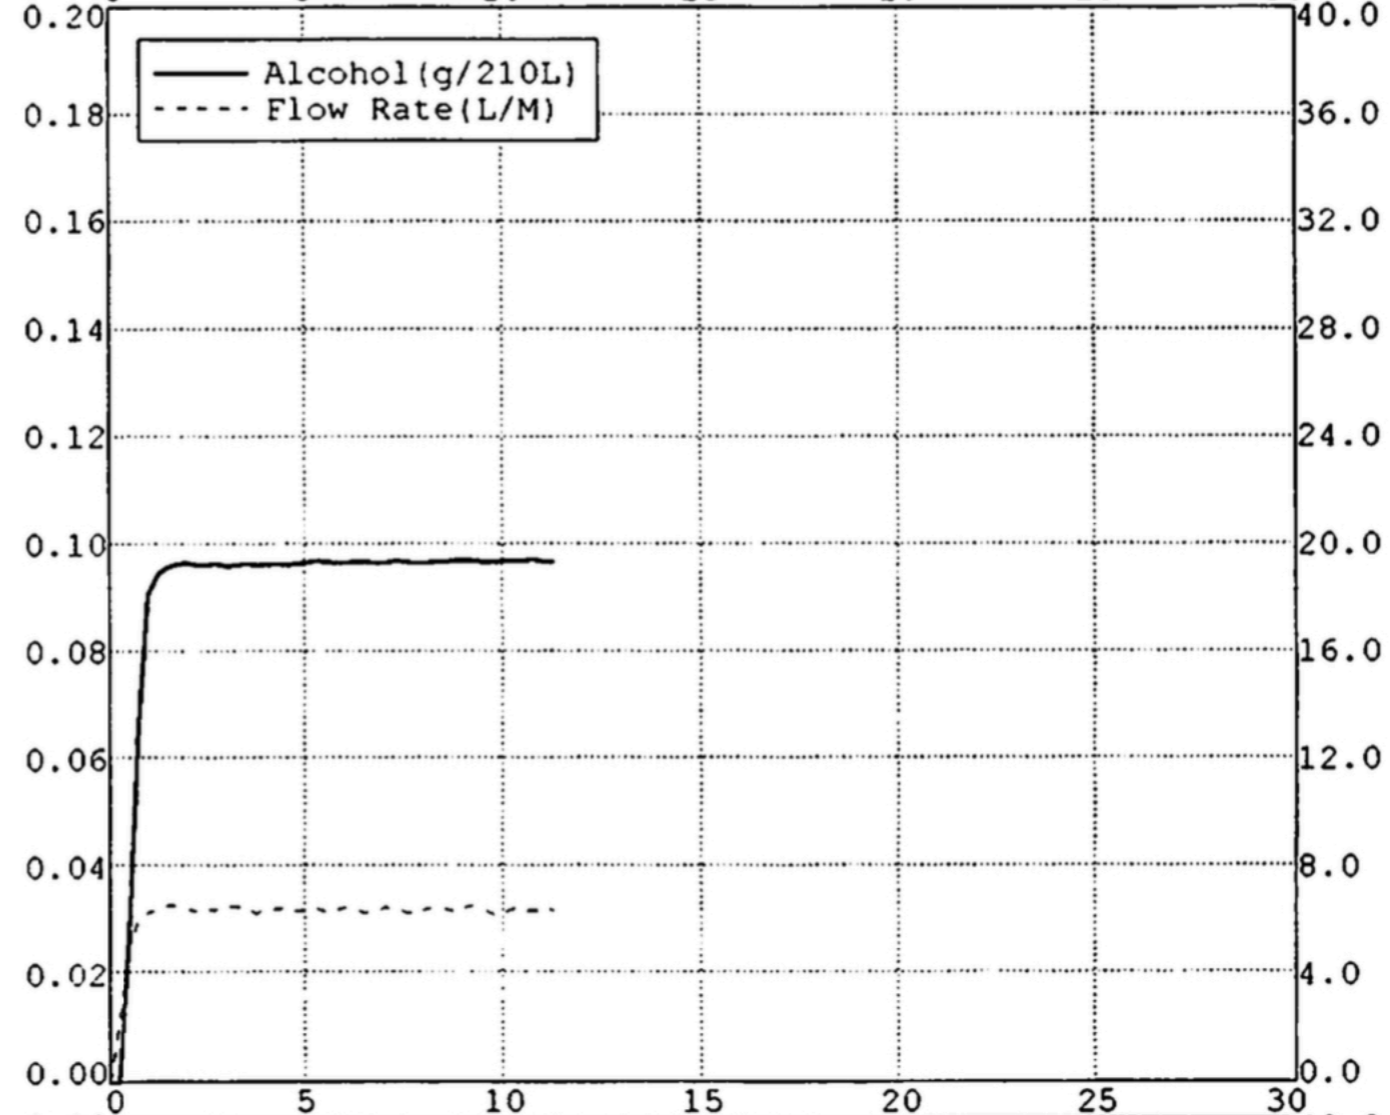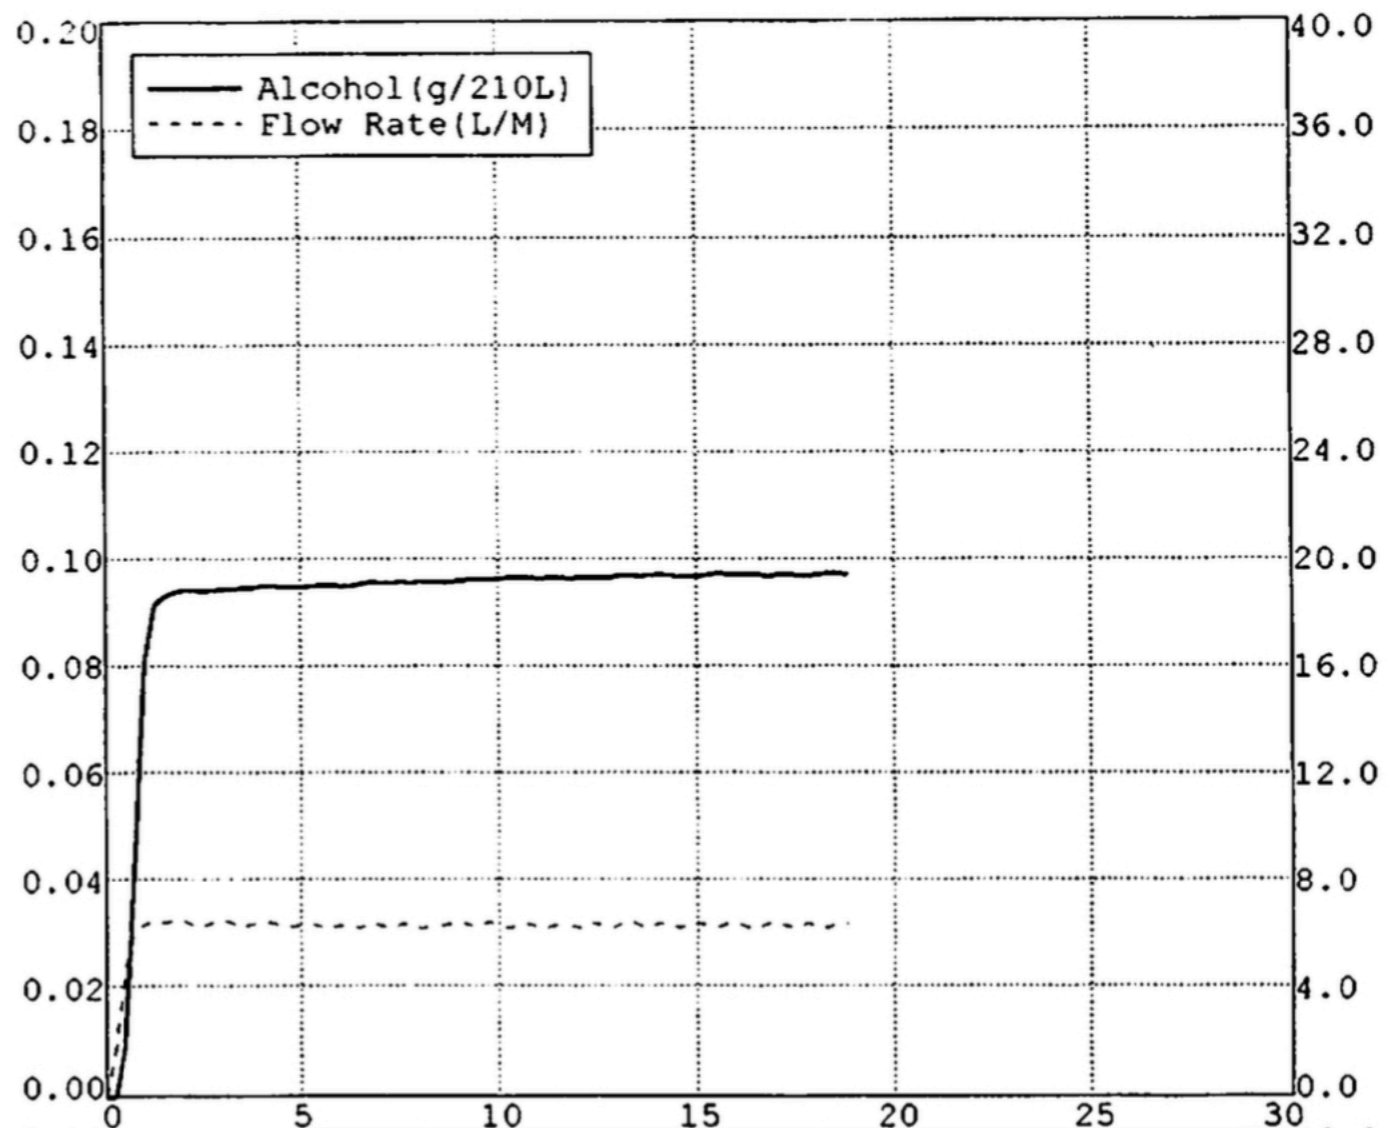

▼↑⊙↑ -◆↑Ç-▶