

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606




LEB

Date: 05/18/2022

OPERATOR NAME:
JOHN P CUSACK
Permit #: 35563
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:44
INTERNAL STANDARD	VERIFIED	20:44
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	20:44
BLANK TEST	0.00	20:45
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	20:45
BLANK TEST	0.00	20:46
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	20:46
BLANK TEST	0.00	20:47

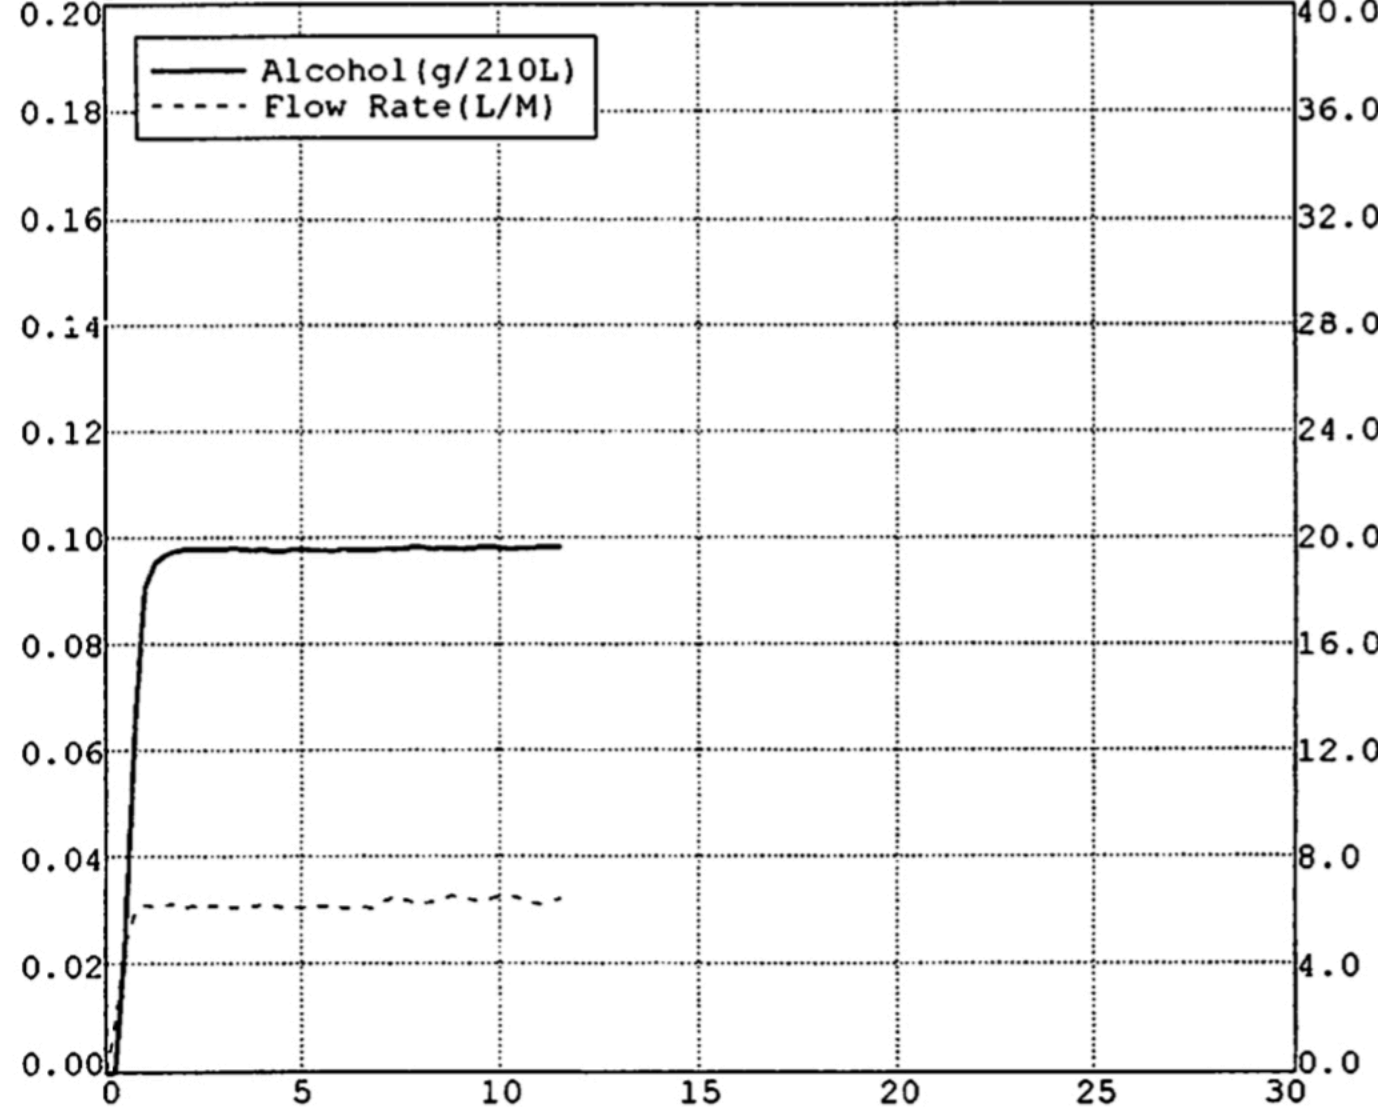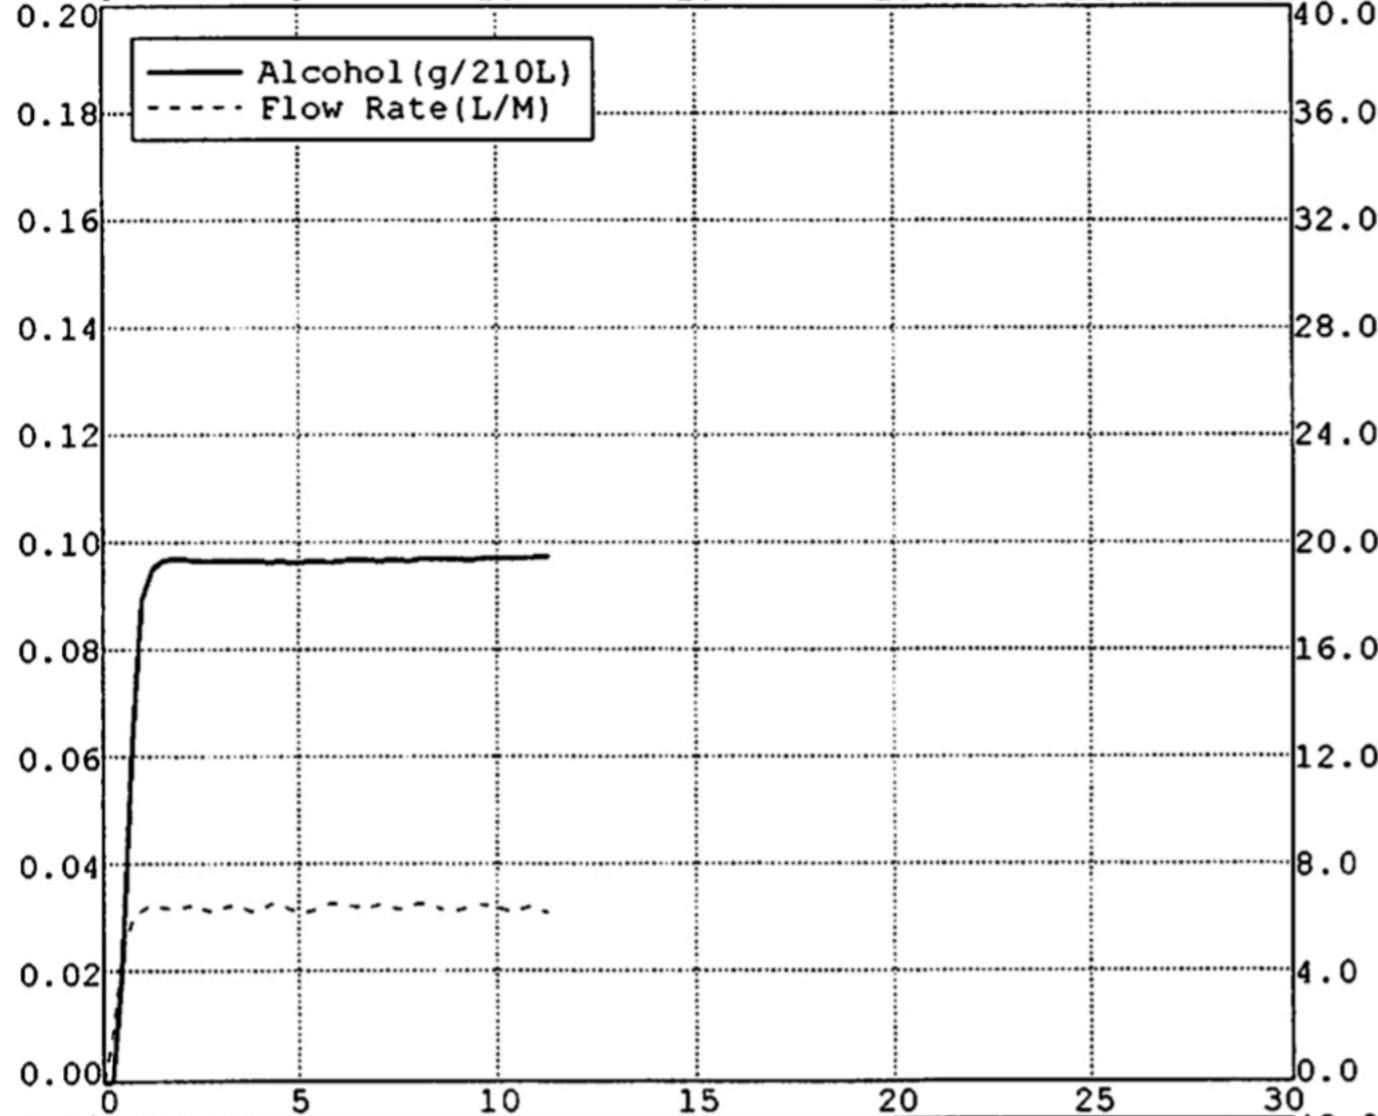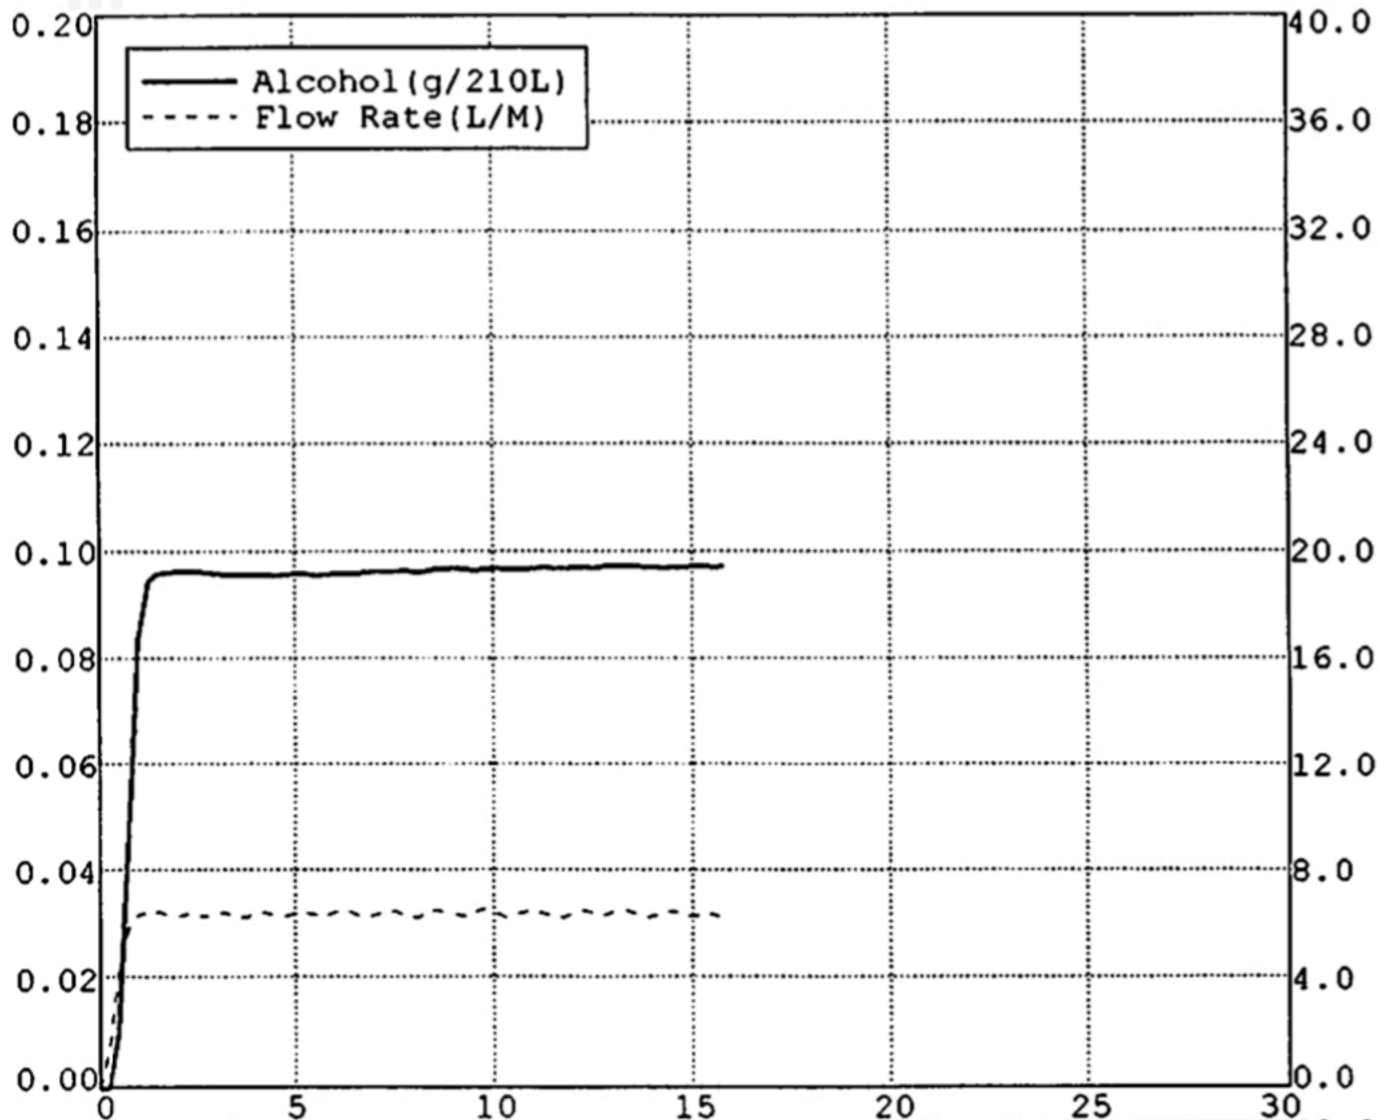

b3W~H