

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606




LEB

Date: 10/04/2023

OPERATOR NAME:
JOHN P CUSACK
Permit #: 35563
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:03
INTERNAL STANDARD	VERIFIED	19:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	19:03
BLANK TEST	0.00	19:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	19:05
BLANK TEST	0.00	19:06
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	19:06
BLANK TEST	0.00	19:07

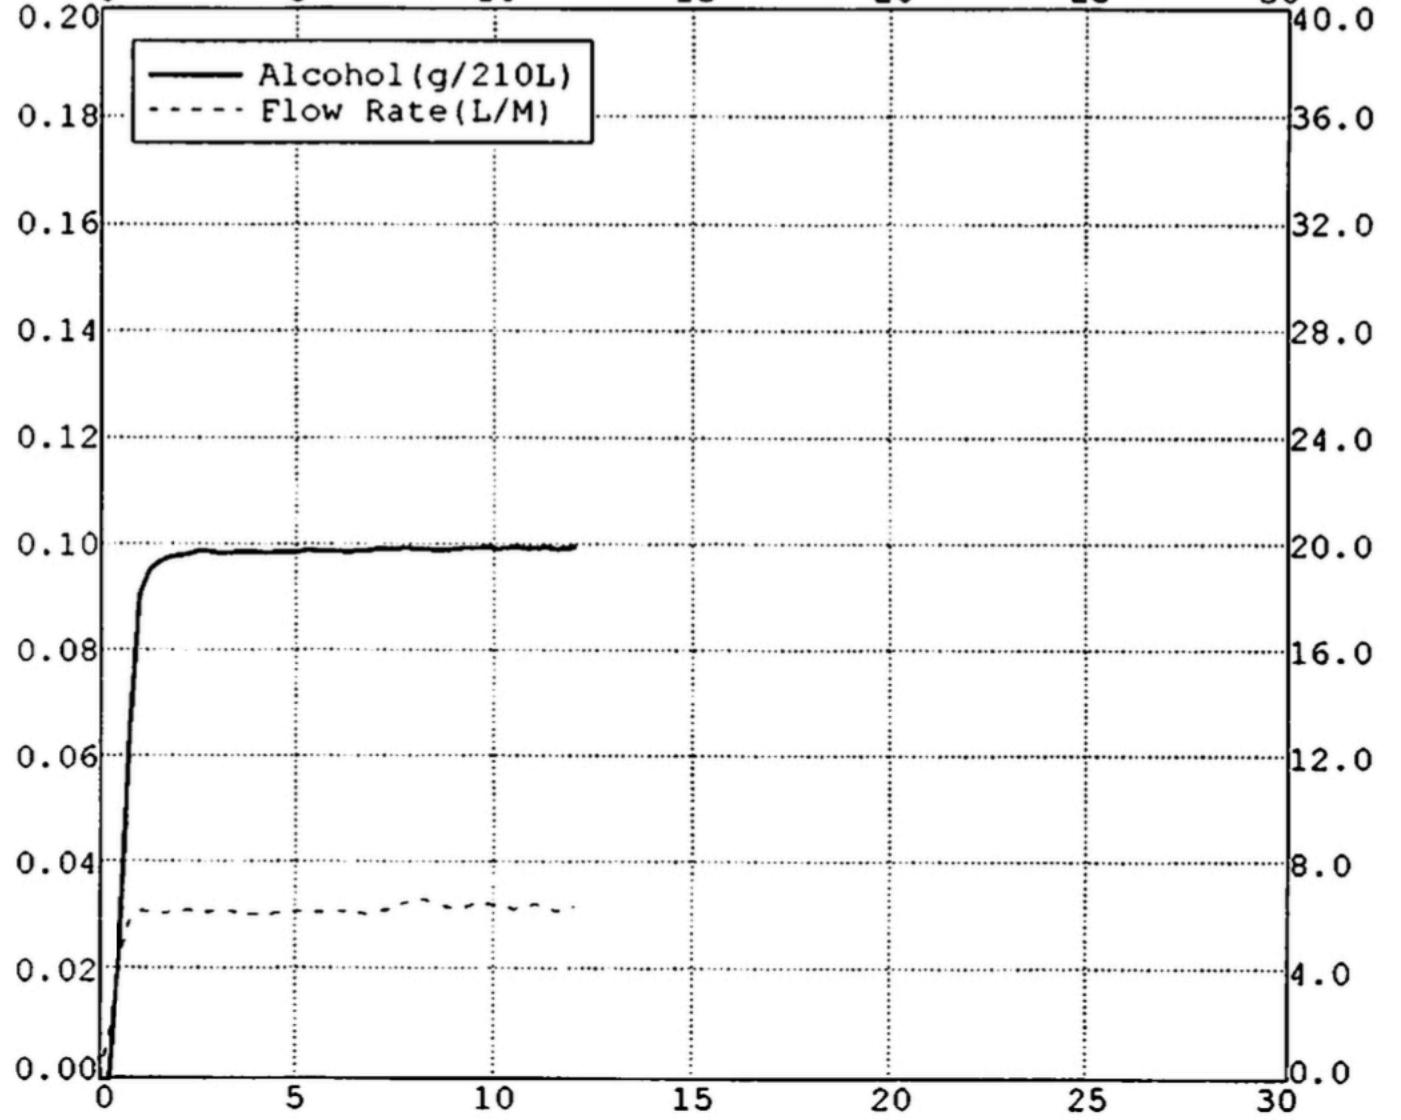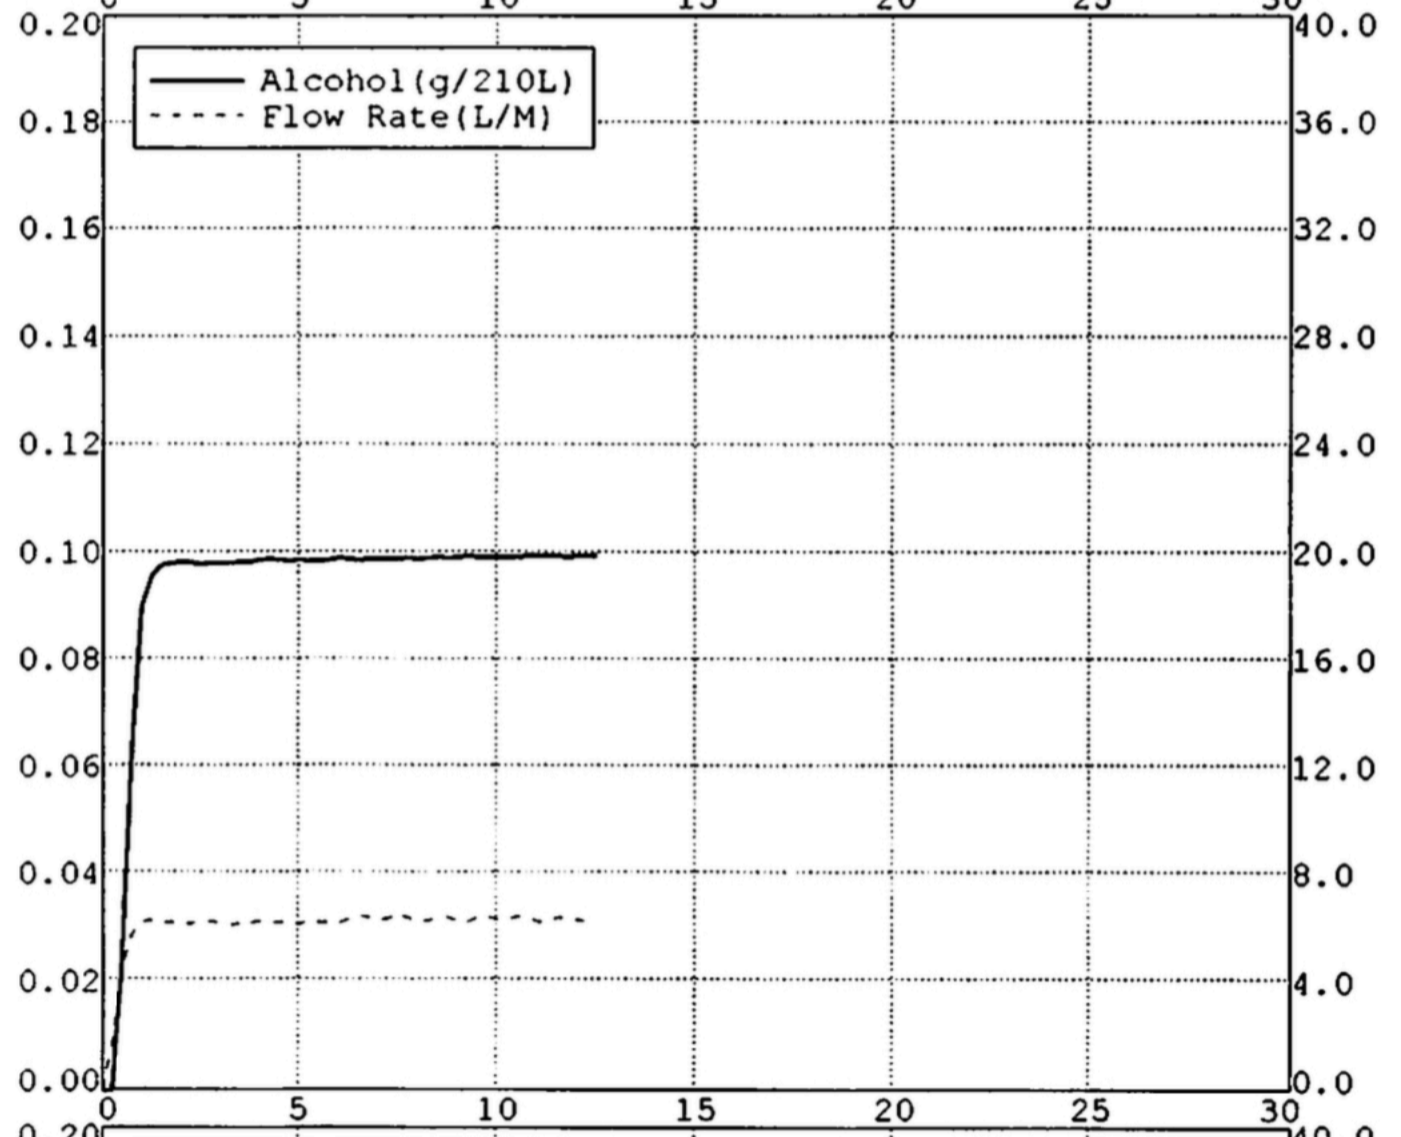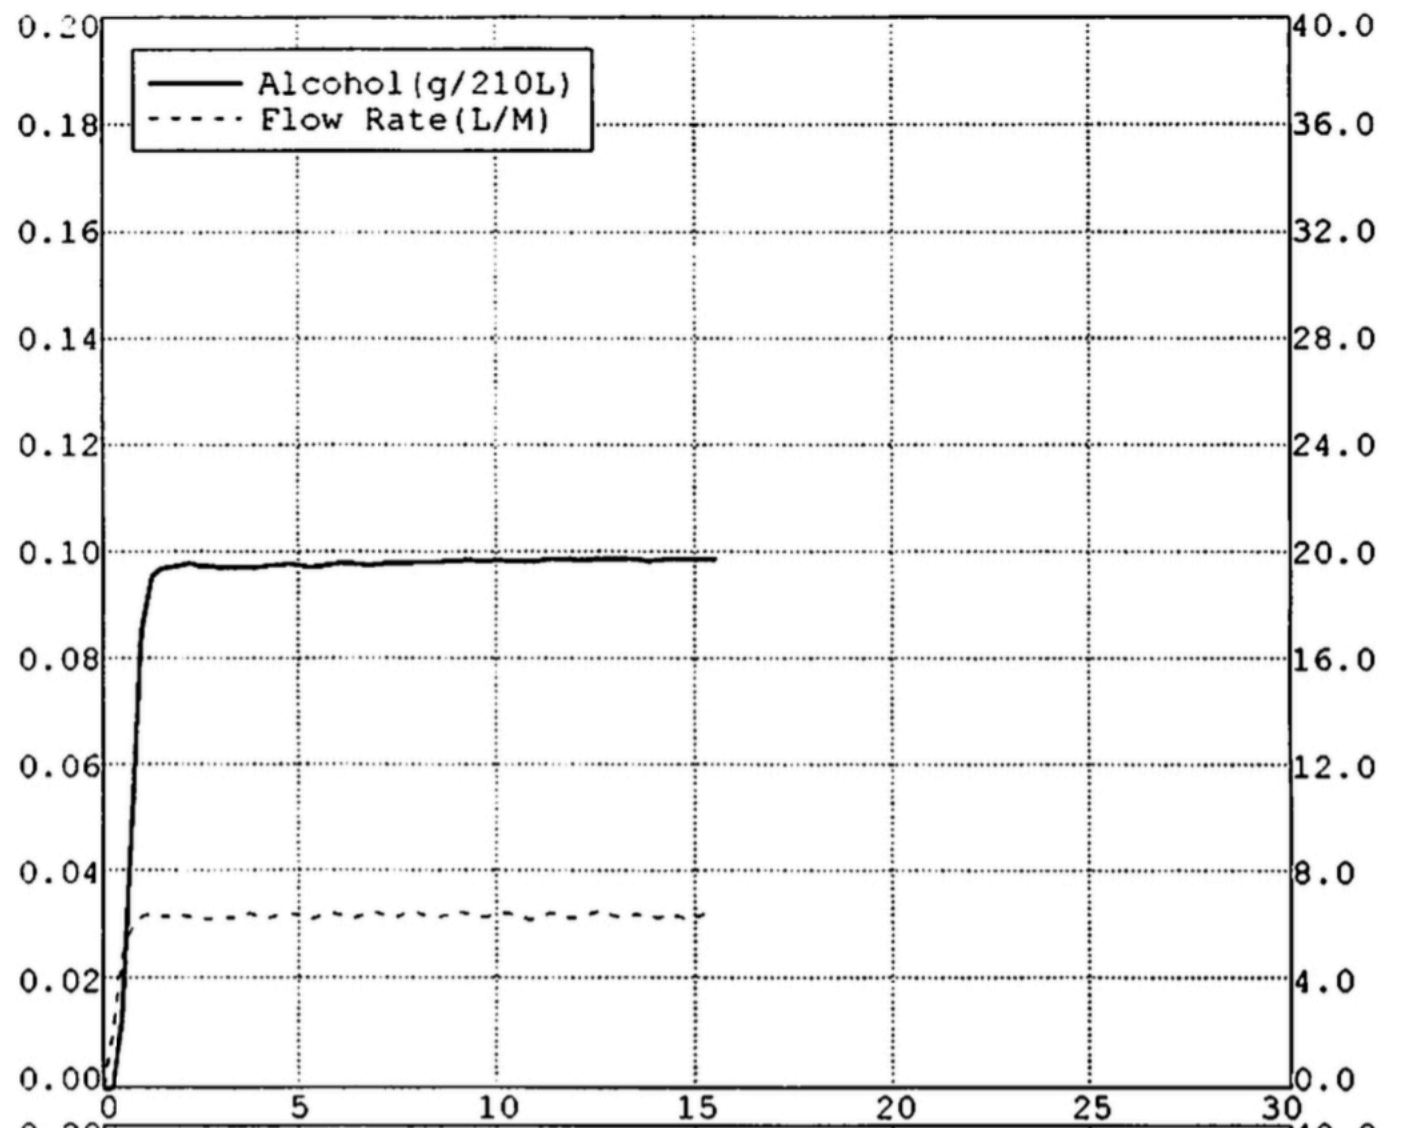

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 10/04/2023

LEB

OPERATOR NAME:
JOHN P CUSACK
Permit #: 35563
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 23270

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:03
INTERNAL STANDARD	VERIFIED	19:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	19:03
BLANK TEST	0.00	19:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	19:05
BLANK TEST	0.00	19:06
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	19:06
BLANK TEST	0.00	19:07

