

SUPERVISOR TEST


ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 113606

Date: 07/08/2026

OPERATOR NAME:
BRADY A WOOD
Permit #: 52004
Operator Agency/Dept: ONEIDA CO. SO
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:17
INTERNAL STANDARD	VERIFIED	03:18
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	03:18
BLANK TEST	0.00	03:19
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.09	03:19
BLANK TEST	0.00	03:20
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	03:20
BLANK TEST	0.00	03:21

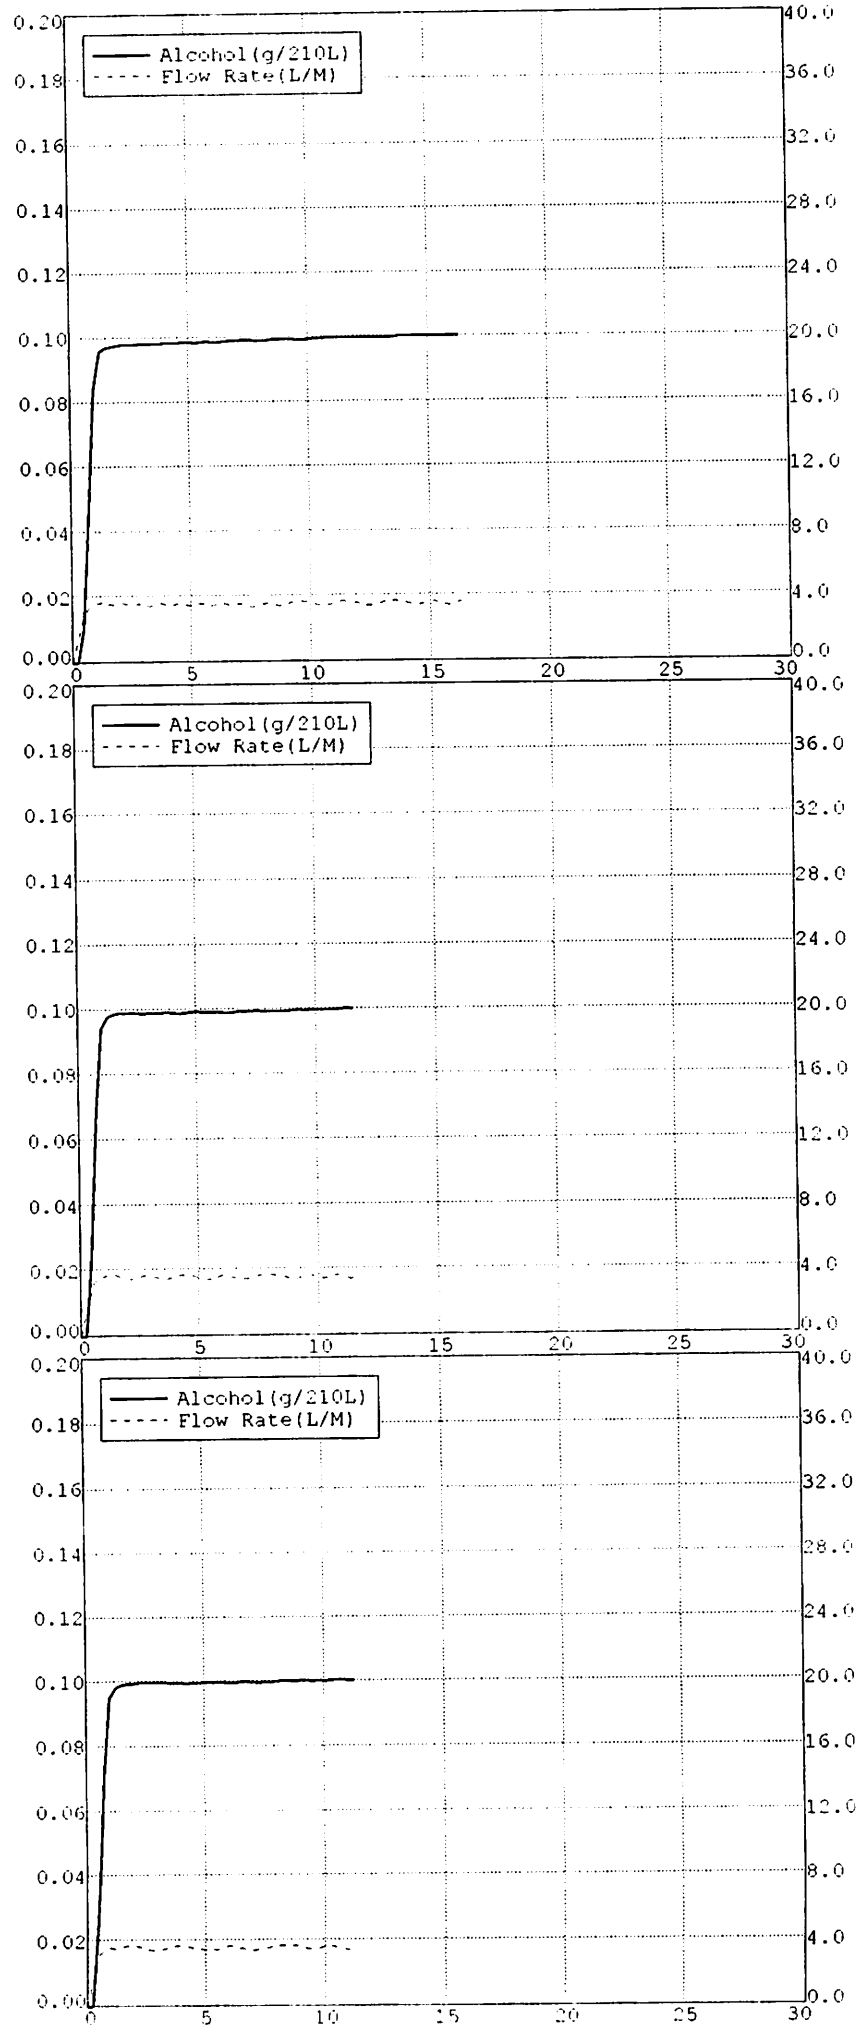

LEB

[Signature] 66
7/8/26