

SOLUTION CHANGE




ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197

Date: 07/31/2021

OPERATOR NAME:
JASON L OSIKA
Permit #: 35567
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:49
INTERNAL STANDARD	VERIFIED	23:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	23:50
BLANK TEST	0.00	23:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	23:51
BLANK TEST	0.00	23:52
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.10	23:52
BLANK TEST	0.00	23:53

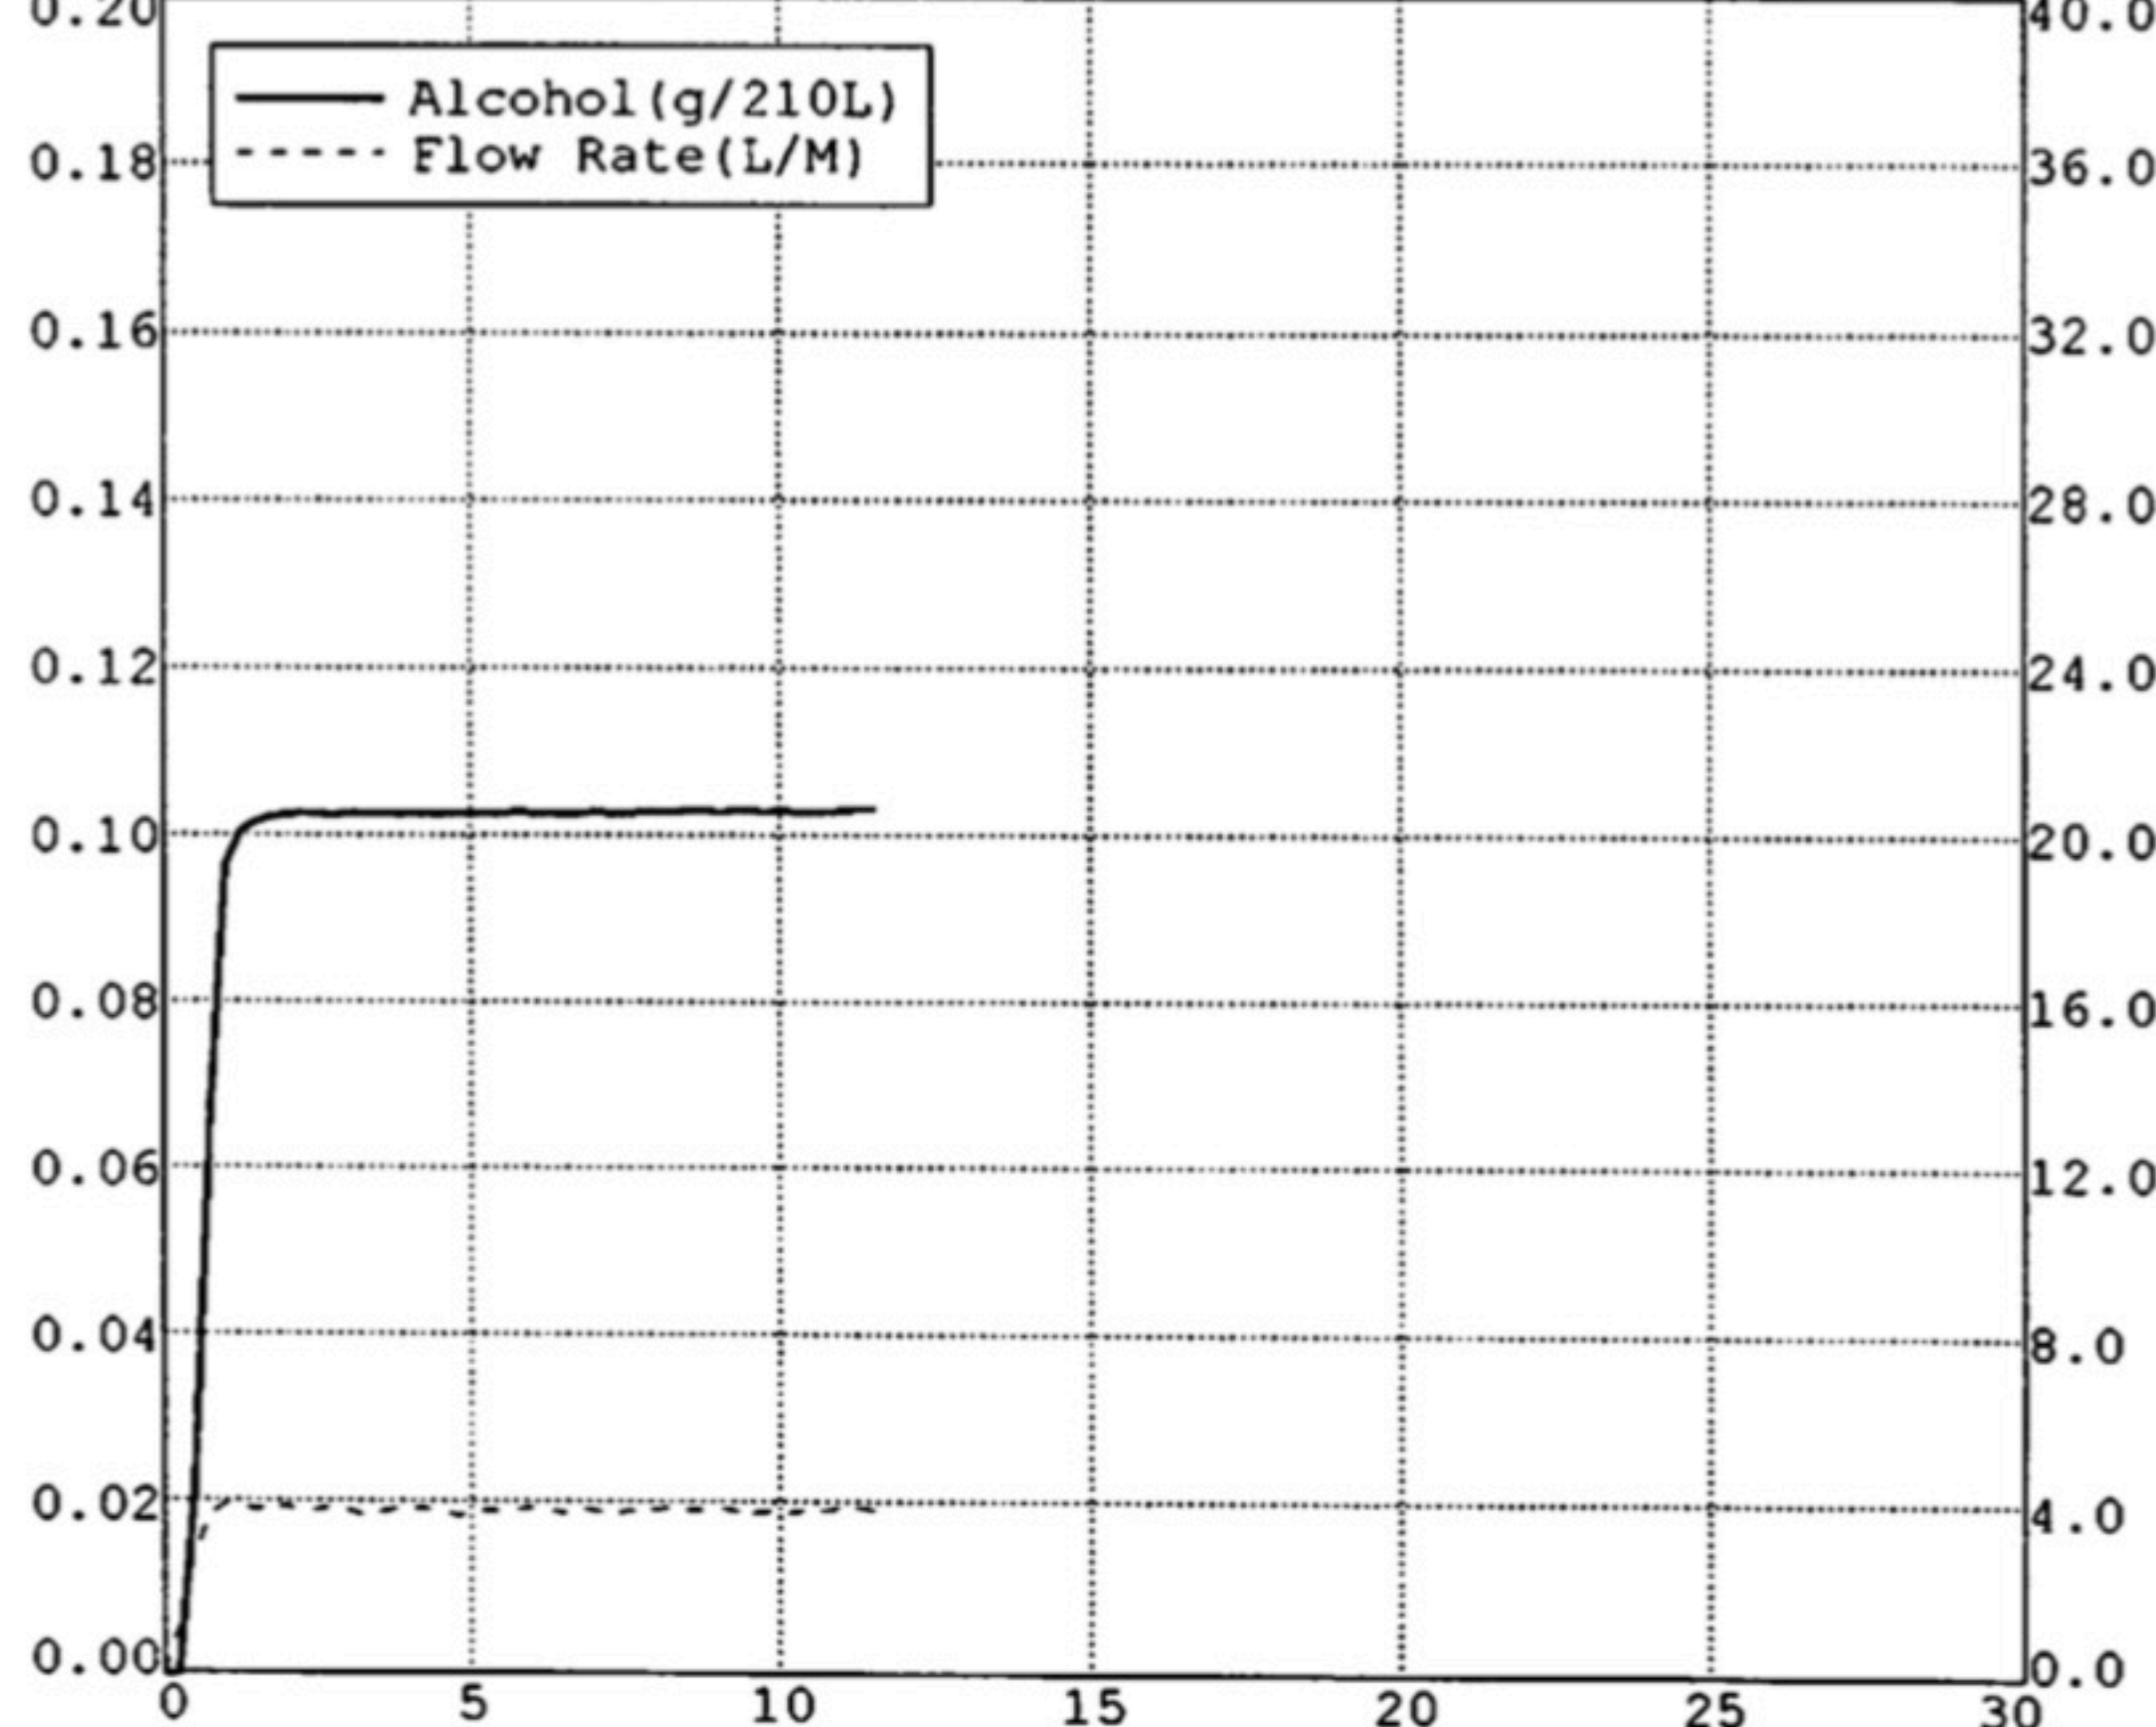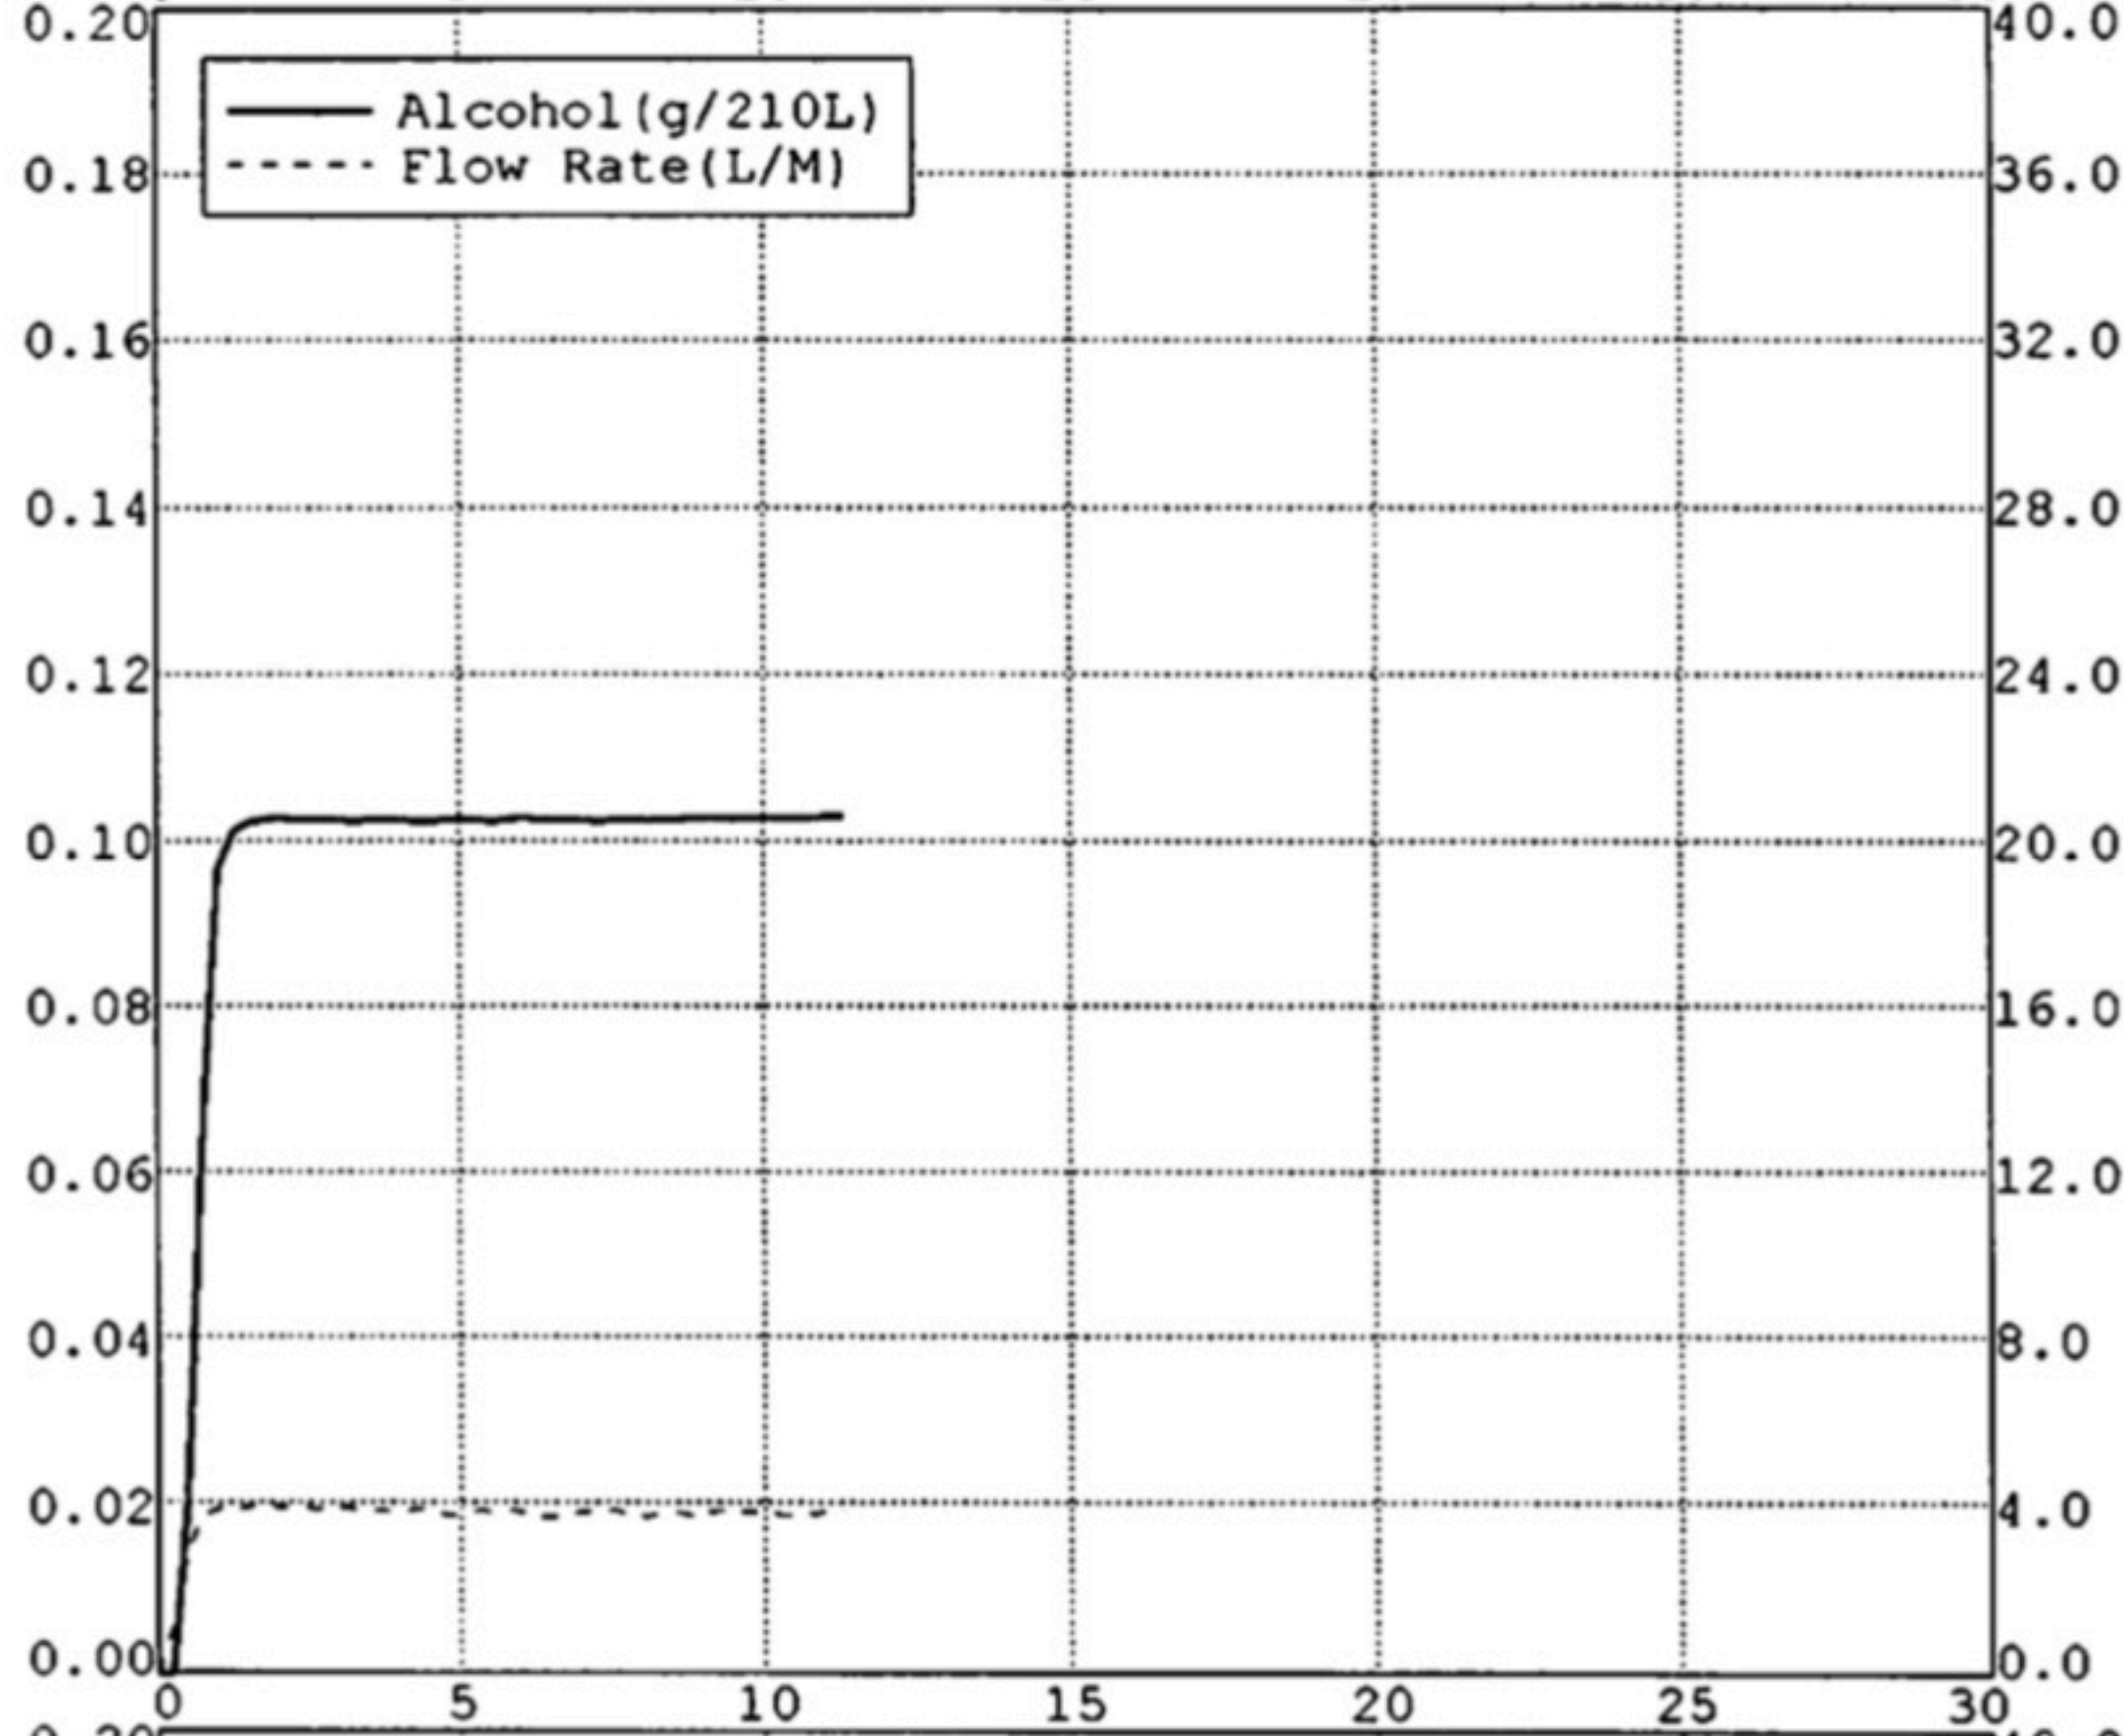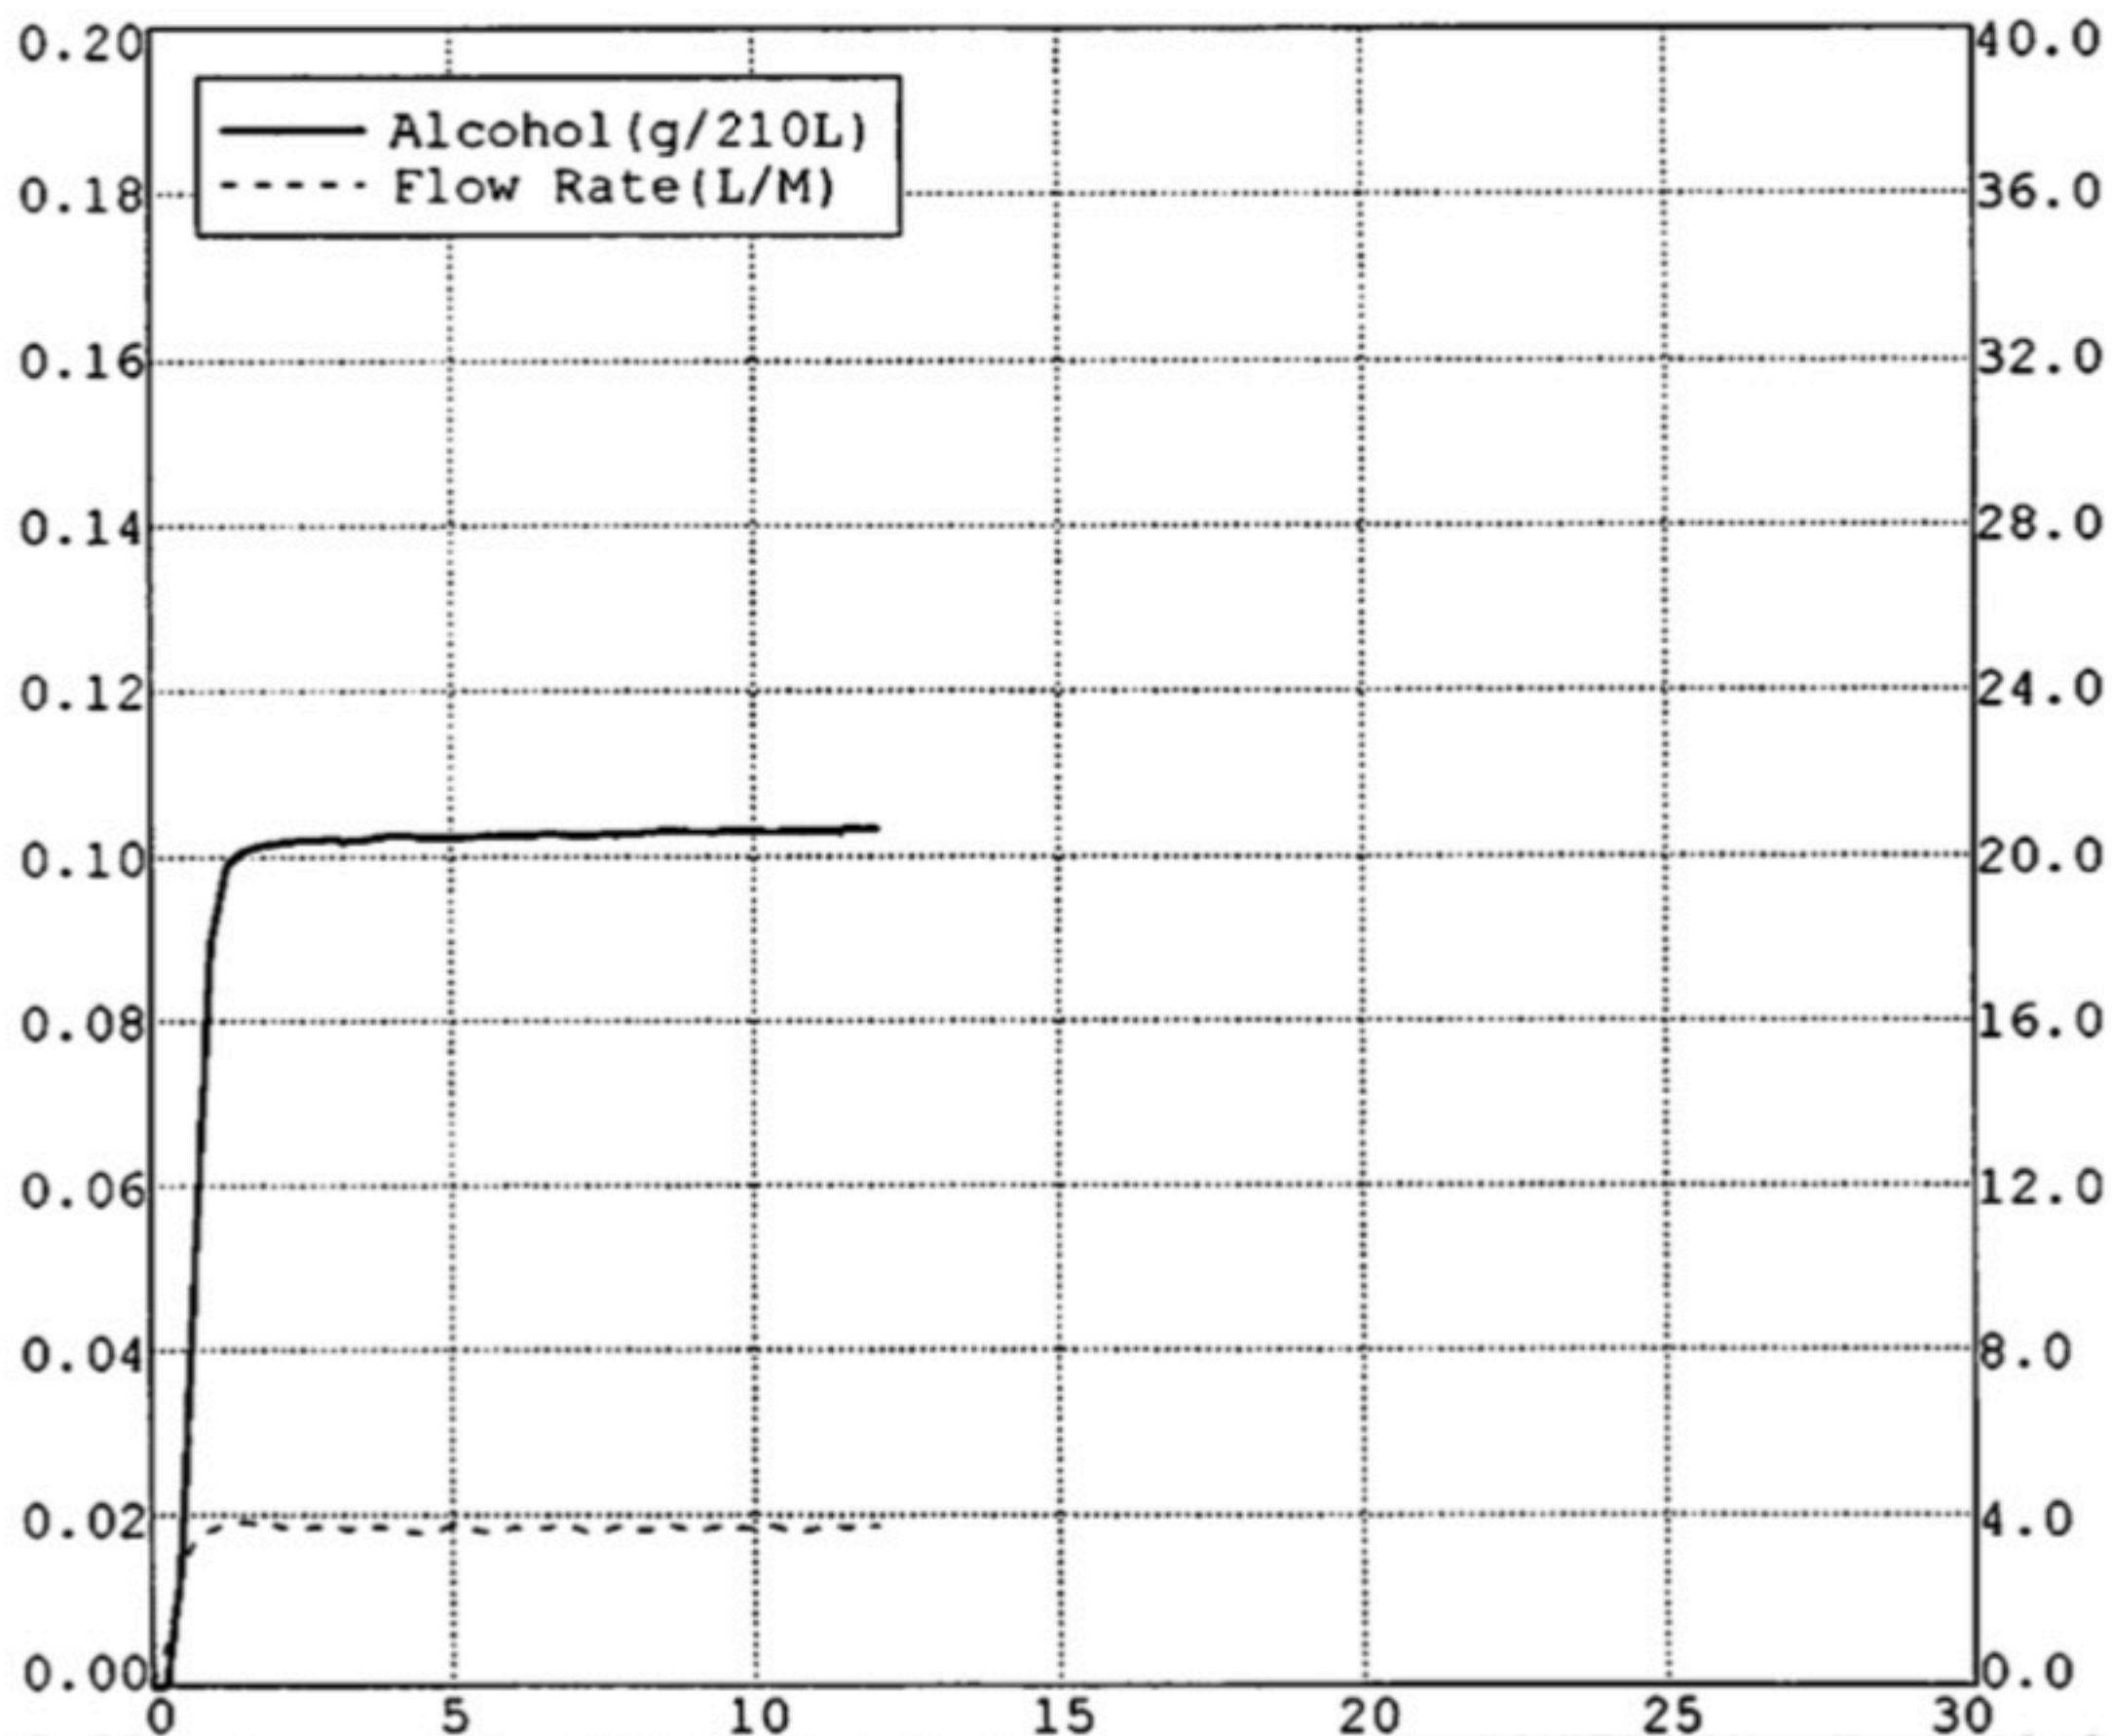

SUPERVISOR TEST

ONEIDA COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 100197

Date: 08/04/2021

OPERATOR NAME:
STEVEN P EILERS
Permit #: 49321
Operator Agency/Dept: ONEIDA CO. S.O.
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:05
INTERNAL STANDARD	VERIFIED	22:05
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:05
BLANK TEST	0.00	22:06
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:06
BLANK TEST	0.00	22:07
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:08
BLANK TEST	0.00	22:08

