

SUPERVISOR TEST

ONEIDA COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 100197

WFO



Date: 08/23/2023

OPERATOR NAME:  
JOHN P CUSACK  
Permit #: 35563  
Operator Agency/Dept: ONEIDA CO. S.O.  
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:34
INTERNAL STANDARD	VERIFIED	21:34
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	21:35
BLANK TEST	0.00	21:35
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	21:36

RFI Detected

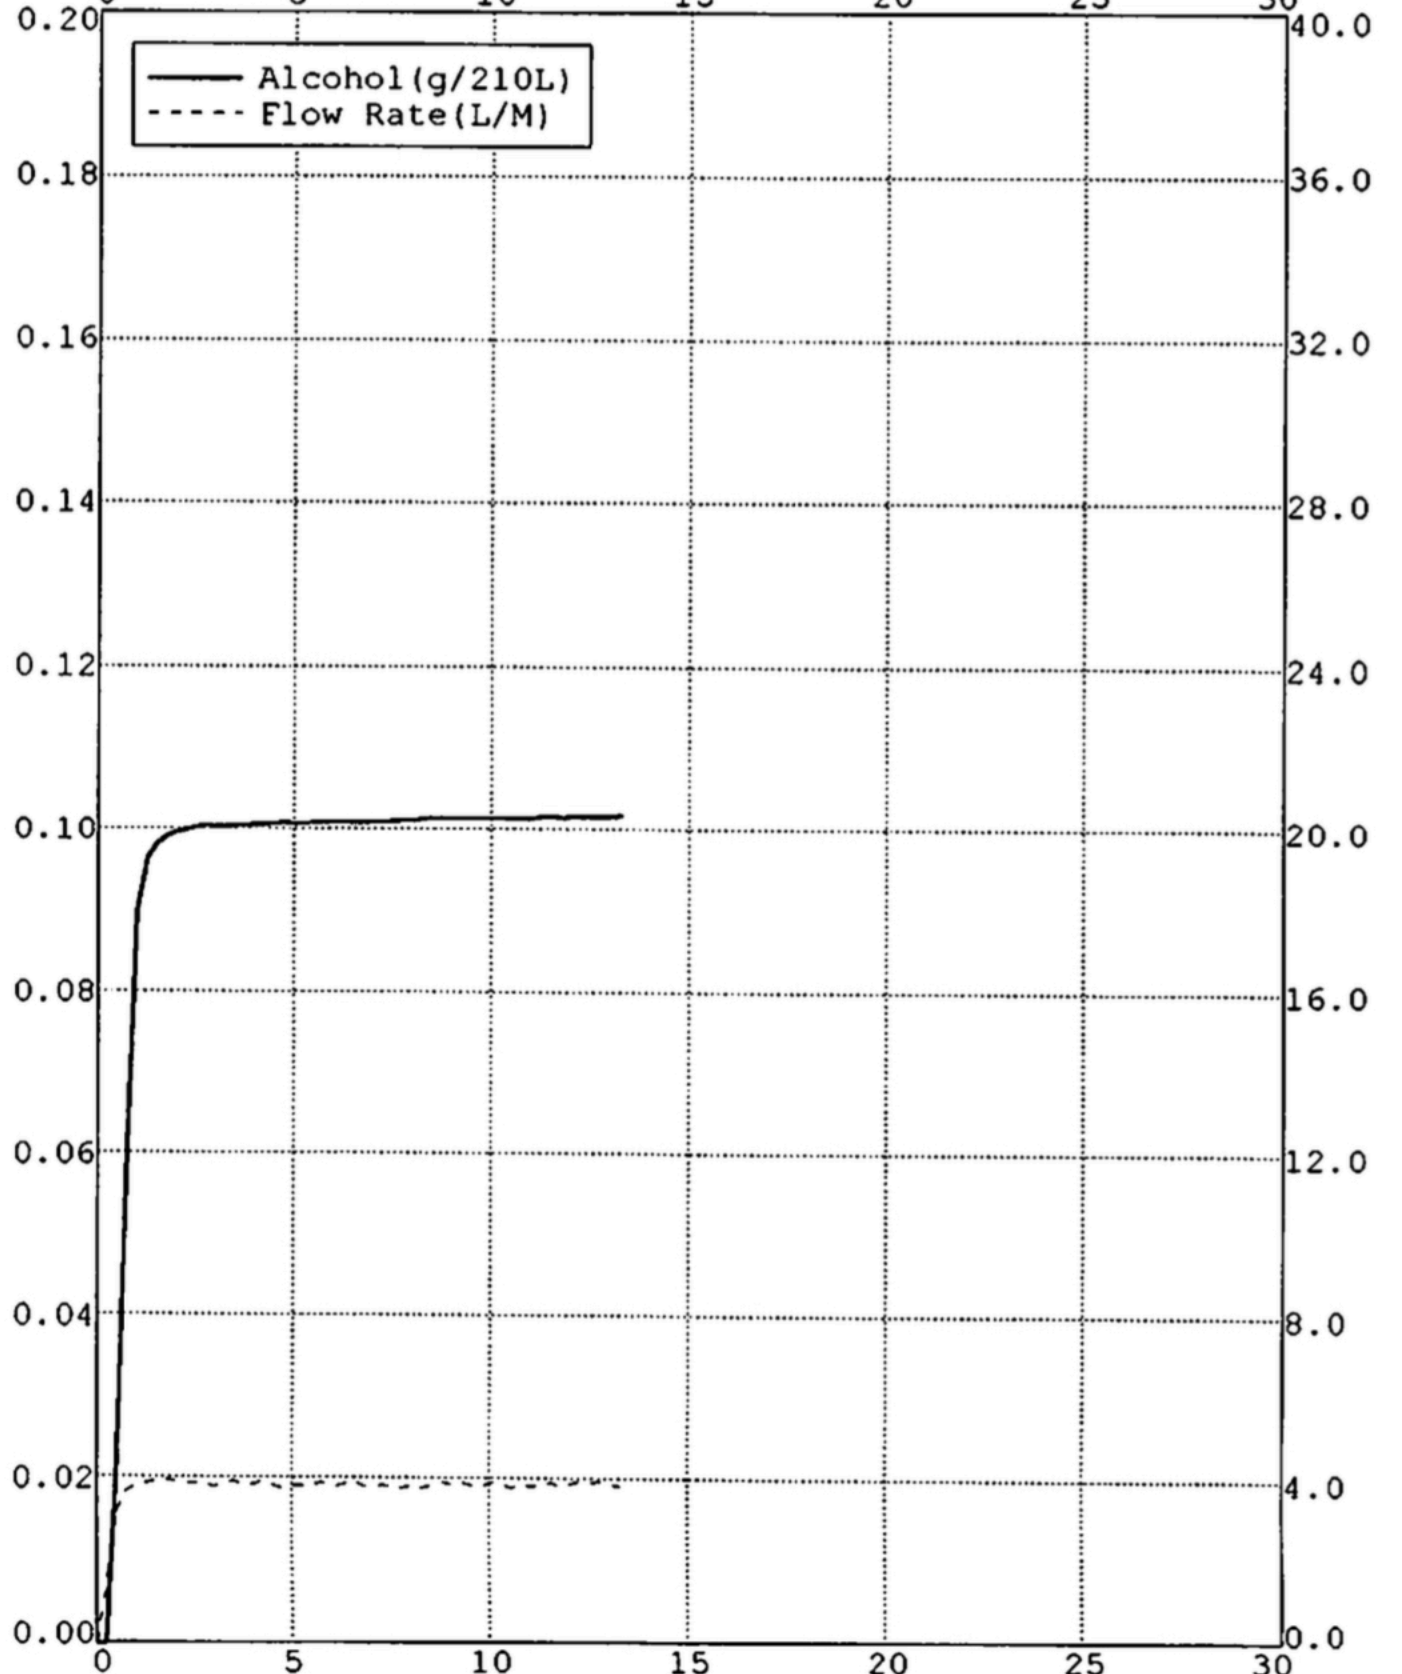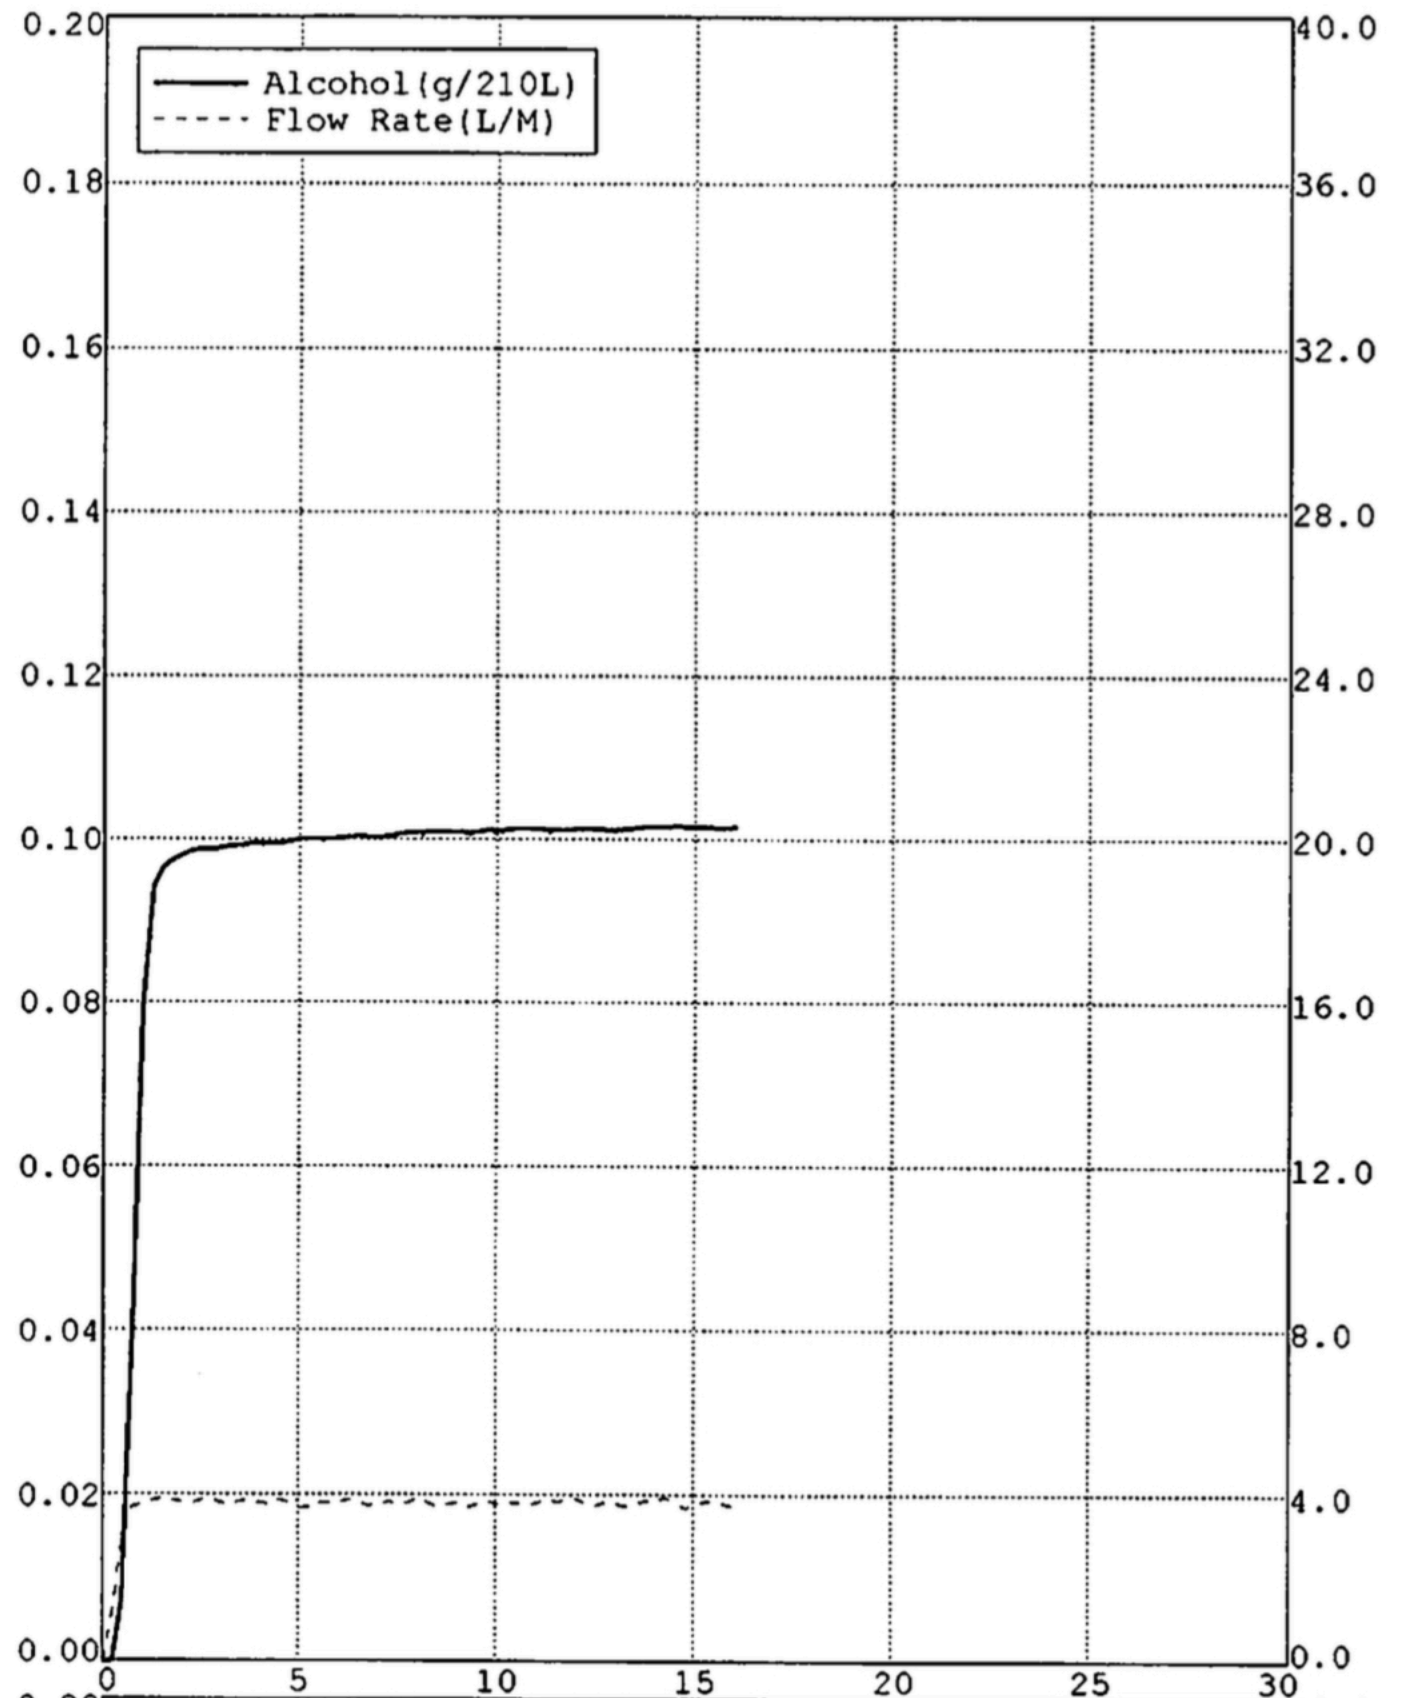

SUPERVISOR TEST

ONEIDA COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 100197

WFO

Date: 08/23/2023

OPERATOR NAME:  
JOHN P CUSACK  
Permit #: 35563  
Operator Agency/Dept: ONEIDA CO. S.O.  
Reference Standard #: 23190

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:39
INTERNAL STANDARD	VERIFIED	21:39
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	21:40
BLANK TEST	0.00	21:41
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	21:41
BLANK TEST	0.00	21:42
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	21:42
BLANK TEST	0.00	21:43

